



Cardiovascular Suite

Cardiovascular Suite 4.5.0

User Manual and Instructions For Use

Document number: TEC0002EN Rev.20

March 30th, 2022

Cardiovascular Suite is a software for the estimation of early markers of cardiovascular risk by ultrasound imaging of the vessel longitudinal section. In particular, the software is composed of two main modules of measurement: 1) the FMD-Studio for the measurement of Flow-Mediated Dilation (FMD) of the brachial artery, by processing sequences of ultrasound images; 2) the Carotid-Studio for measuring the Intima-Media Thickness (IMT) and the diameter of the carotid artery by processing sequences of ultrasound images that, when combined with an estimate of pressure, provides parameters of arterial elasticity. On single images, the software provides also a tool for the measurement of geometric and statistic parameters on portions of the image that are recognized manually by the operator as plaques. The system is able to process images (or sequences of images) recorded on files, or can process in real-time the video output of an ultrasound system.

In accordance with the rules of application of chapter 1.4 of Annex IX of the European Directive 93/42/EEC and subsequent amended and the provisions of Chapter III of Annex IX of the European Directive 93/42/EEC and subsequent amendments, Cardiovascular Suite software is within the medical devices of Class IIa according to rule 10. The product is in compliance with the legal requirements of the European Directive 93/42/EEC and subsequent amendments and supplements (European Directive 2007/47/EC) for medical devices. This software is not to be used in any country without appropriate regulatory clearance, license, or registration as may be required by in country regulatory agencies.

The product labeling for the Cardiovascular Suite is comprised of the Manual and Instructions for Use, the login screen of the software as well as in the product license key, and product package leaflets.

A printed version of the User Manual and Instruction for Use can be requested at support@quipu.eu.

Adobe Acrobat Reader ver. 6 or later is recommended to correctly display the PDF version of the User Manual and Instruction for Use.

CE⁰⁴⁷⁶
Rx Only



QUIPU SRL
via Moruzzi 1, 56124 Pisa - Italy
+39.050.3152612 support@quipu.eu

Table of Contents

1	Indications for Use & Safety Information.....	5
2	Recommendations.....	8
3	Installation	9
3.1	System requirements.....	9
3.2	Apple computer.....	10
3.3	Microsoft Windows computer	11
3.4	Archive folder	14
3.5	Moving to a new computer	15
3.6	Extraordinary maintenance.....	16
3.7	Decommissioning and disposal	16
4	License	18
4.1	Activating a license	19
4.2	Evaluation license	21
4.3	License manager	24
5	Image and video sources	26
5.1	Using image or video clip for offline analysis	26
5.2	Video and image player	26
5.3	Connecting your computer to the ultrasound system	28
5.4	How to set up the ultrasound system	35
6	Login	40
7	Home	41
8	Settings manager	42
8.1	General settings	42
8.2	Carotid Studio settings	43
8.3	FMD Studio settings	43
9	Archive	45
9.1	STUDIES AND DOCUMENTS	45
9.2	PATIENTS	45

9.3 OPERATORS.....	46
9.4 INSTITUTES	46
9.5 PROTOCOLS	46
9.6 TAGS.....	47
9.7 Studies management.....	47
9.8 Patients management	53
9.9 Operators management	56
9.10 Institutes management	58
9.11 Protocols managements	60
9.12 Tags management	62
10 Carotid Studio	64
10.1 Create a new study.....	64
10.2 Cineloop study analysis.....	71
10.3 Single image study analysis.....	79
10.4 Calibrate the B-mode image.....	86
10.5 Cineloop study review	87
10.6 Single image study review	96
10.7 Study report	101
11 FMD Studio	104
11.1 Create a new study.....	104
11.2 Analysis.....	110
11.3 Review	124
12 Warnings.....	136
13 References.....	137
14 Contacts.....	139
15 Notes.....	140
15.1 Trademarks	140
15.2 EULA.....	140
15.3 Privacy policy	146
15.4 Open source	151



15.5 LGPL 2.1	152
15.6 LGPL 3	157



1 Indications for Use & Safety Information

Please read all following instructions, precautions, and warnings carefully before use.

Indications for Use

The Cardiovascular Suite is a software program that is intended to aid trained healthcare practitioners in the quantitative analysis of vascular ultrasound images, particularly for the measurement of the diameter and its changes on the brachial artery, the diameter and its changes on the carotid artery, the Carotid Intima-Media Thickness, and for carotid plaque analysis.

Contraindications

The Cardiovascular Suite device is not intended for use as a test that provides a direct diagnosis of any cardiovascular disease. It is intended to supplement, not substitute, the physician's decision-making process for diagnosis and treatment. It should be used in conjunction with knowledge of the patient's history and other clinical findings.

Precautions and Warnings

Below are a list of Precautions and Warnings for the Cardiovascular Suite. All of the following items are found in their appropriate sections throughout this document as well.

Precautions

- CAUTION: the computer must be a Medical Grade Computer in compliance with EN 60601-1 standard for electrical isolation and safety or a common CE marked personal computer (89/366/EEC) connected to power supply via Medical Grade Isolation Transformer that meets IEC 60601-1 standard for electrical leakage.
- CAUTION: The operating system of the machine where the software is used requires controlled access with user name and password. In addition, a time-out of 15 minutes is recommended in the user session of the operating system where the software runs.
- CAUTION: The operating system where the software runs must be updated.
- CAUTION: An updated antivirus/antimalware software protection should be present in the computer where the software runs.
- CAUTION: If the computer is connected to the network, a firewall should be used to prevent cyber-attacks.
- CAUTION : The Quipu License Key contains your license. Store it in a safe place in order to avoid loss and / or theft.
- Please, note that an Internet connection is needed to obtain and use the Evaluation License
- CAUTION: The B-mode window in the image must have a minimal resolution of 6 pixels/mm. If present, the size of the PWD window in the image must be at least 200x100 pixels.
- CAUTION: The ultrasound device must be suitable for vascular imaging and it must be equipped with a vascular linear probe with frequency greater than 5MHz.
- CAUTION: The ultrasound scanner must be in accordance with the European Medical Device Directive 93/42/EEC or cleared / registered / licensed by the appropriate regulatory authority.
- CAUTION: If the video converter is used with an AC/DC power adapter, it must be a medical grade power adapter according to IEC 60601-1, current edition.
- CAUTION: The video converter must be connected directly to a USB port on your computer. Do not use hubs or the USB socket on the external keyboard. Use USB 3.0 to maximize performances.
- CAUTION: verify that the video output type and resolution of the ultrasound scanner are compatible with this video converter.
- CAUTION: the AV.io HD must be updated with the last firmware from Epiphan System Inc.
- CAUTION: the video converter must be connected directly to a USB port on your computer. Do not use hubs or the USB socket on the external keyboard. Use USB 3.0 to maximize performances.
- CAUTION: Exclude any noise reduction filter (especially temporal filters).
- CAUTION: pay attention that nothing but the ultrasound image is into the ROI. Please note that the processing can be affected by annotations or any other graphical object that is superimposed to the image. In particular, pay attention that the cursor of the doppler sample volume is not into the ROI.

- CAUTION: the processing can be affected by annotations or any other graphical object that is superimposed to the image into the Doppler Flow ROI.
- CAUTION: the data produced by Cardiovascular Suite are not deleted during the software uninstall procedure. They should be removed manually by deleting the archive folder.
- CAUTION: the backup of the archive folder is recommended before uninstalling/installing the software.

Warnings

- CAUTION: Failure / incomplete / incorrect installation makes it not possible to use the software.
- CAUTION: It is recommended to perform regular backups of the system. The non-operation of the backup could result in permanent data loss.
- CAUTION: if a virus/malware is detected in the computer where the software runs the user should adopt the suitable countermeasures that can include removing our software and re-installing it.
- CAUTION : The Quipu License Key will work only on the computer where it is used for the first time.
- CAUTION: the lack of calibration can generate a software malfunction.
- CAUTION: the processing can be affected by annotations or any other graphical object that is superimposed to the image into the Doppler Flow ROI.






Labeling

The product labeling for the Cardiovascular Suite is comprised of the Manual and Instructions for Use, the login screen of the software as well as in the product license key, and product package leaflets.

Below is a table of all labeling symbols for the Cardiovascular Suite.

Labeling Symbols Table

Symbol	Meaning
R_x Only	Prescription Only: Caution: U.S Federal law restricts this device to sale by or on the order of a physician or health care practitioner.
	Product Model Number / Reference Number
	Manufacturer information
	Year of Manufacture

	<p>Caution. Indicates the need for the user to consult the instructions for use for important cautionary information such as warnings and precautions that cannot, for a variety of reasons, be presented on the medical device itself.</p>
	<p>Consult instructions for use</p>
	<p>CE Mark (Conformité Européenne).</p> <p>The product is in compliance with the legal requirements of the European Directive 93/42/EEC and subsequent amendments and supplements (European Directive 2007/47/EC) for medical devices.</p>
	<p>Do not store below 5°C or above 55°C</p>
	<p>Do not store below 5% humidity or above 95% humidity.</p>

2 Recommendations

⚠ CAUTION : This manual describes the instructions for proper use of the device software Cardiovascular Suite. Please carefully read the advice in this document.

The software must be used by trained and qualified personnel, such as laboratory technicians, nurses, physicians and / or sonographers, who have experience in acquisition and analysis of vascular ultrasound images. It is recommended that the user is aware of the meaning of the parameters measured and returned as a result from the device. It is recommended that the operator does not have serious problems with vision and hearing. It is required the knowledge of the mother tongue or, for those countries that allow it, of the English language.

A visual impaired due to particular ambient conditions, a visually impaired user, a not optimized brightness, and/or not optimized resolution of the monitor may affect the correct interpretation of the results provided.

The analysis performed by the device can be applied to any adult person who can undergo an ultrasound examination. It is not recommended to use the system for analysis of people with a distorted anatomy of the examined arterial segment.

It is recommended that the device is used according to the international guidelines for estimating carotid biomarkers and brachial flow-mediated dilation (FMD).

The software is installed on a computer and it can be used in conjunction with an ultrasound device and a video converter. For the correct operation it is advisable to pay attention to environmental influences that may alter the operation of these devices. Moreover, it is recommended: i) to adopt the necessary actions in order to prevent virus and malware and ii) to perform periodical data backup. For details, refer to the instructions provided by individual producers.

The software is licensed by a USB dongle key. Use the USB dongle key in an environment with the following conditions of temperature and humidity: operating temperature: +5 ... +55 ° C (+41 ... +131 ° F), humidity: 5 ... 95%. We recommend that you do not expose the USB dongle key to solvents and flammable media. It is recommended to protect the USB dongle key by physical damages.

When you use this software, in case that you manage personal sensitive data, you must do it accordingly to the General Data Protection Regulation UE 2016/679. Sensitive data must be processed in a manner that ensures appropriate security of personal data including protection against unauthorized or unlawful processing and against accidental loss, destruction, or damage, using appropriate technical or organizational measures.



3 Installation

Cardiovascular Suite can be installed on Apple computer or on Microsoft Windows computer. Please see the minimum [System requirements](#) of the computer for a correct execution of Cardiovascular Suite.

⚠ CAUTION: The operating system of the machine where the software is used requires controlled access with user name and password. In addition, a time-out of 15 minutes is recommended in the user session of the operating system where the software runs.

⚠ CAUTION: The operating system where the software runs must be updated.

The software installer can be downloaded from the Quipu website www.quipu.eu

Please follow the correct instruction for the installation of the software on [Apple computer](#) and on [Microsoft Windows computer](#) respectively.

⚠ CAUTION: Failure / incomplete / incorrect installation makes it not possible to use the software.

⚠ CAUTION: It is recommended to perform regular backups of the system. The non-operation of the backup could result in permanent data loss.

⚠ CAUTION: if a virus/malware is detected in the computer where the software runs the user should adopt the suitable contro-measures that can include removing our software and re-installing it.

Once installed, Cardiovascular Suite requires the activation of a [License](#). The license is contained inside a Quipu License Key, which is a USB dongle key. The Quipu License Key must be plugged into the computer where the software is running. Please follow the instruction for [Activating a license](#).

You can ask for a 14-days [Evaluation license](#).

3.1 System requirements

Minimum Requirements

APPLE COMPUTER

- Apple Mac Computer with: Intel Core i5 4th generation 2.3 GHz turbo boost; 4GB RAM; 1GB free Hard Disk space*; 1280x800 monitor resolution.
- Mac OS X 10.12 - 10.15

MICROSOFT WINDOWS COMPUTER

- Intel Core i5 4th generation 2.3 GHz Turbo boost; 4GB RAM; 1GB free Hard Disk space*; 1024x768 monitor resolution.
- OpenGL ES 2.1
- Microsoft Windows 7 64 bit, Windows 8.1 64 bit, Windows 10 64 bit

* 250GB free Hard Disk space is suggested for the Archive

⚠ CAUTION: the computer must be a Medical Grade Computer in compliance with EN 60601-1 standard for electrical isolation and safety or a common CE marked personal computer (89/366/EEC) connected to power supply via Medical Grade Isolation Transformer that meets IEC 60601-1 standard for electrical leakage.

Optional video capture devices for on-line analysis:


- Epiphan - AV.io HD hardware video capture (to connect your computer to DVI, VGA or HDMI video outputs)
- Magewell USB capture AIO (to connect your computer to DVI, VGA, HDMI, S-video and C-video outputs)

3.2 Apple computer


The software installation follows the usual procedure of installing software on Apple computers.

For information or support please contact Quipu support team at support@quipu.eu.

1. Double click on the Cardiovascular Suite disk image file (*.dmg file), a window with the software license will be shown. Read the License Agreement. If you don't accept the license agreement, please click "Disagree" and the installation will quit. If you accept, click the "Agree" button to proceed.

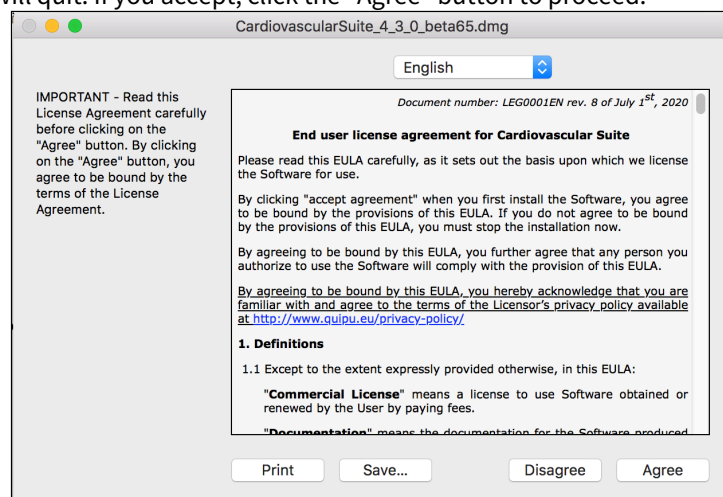

2. Drag the application's icon to your Applications folder.

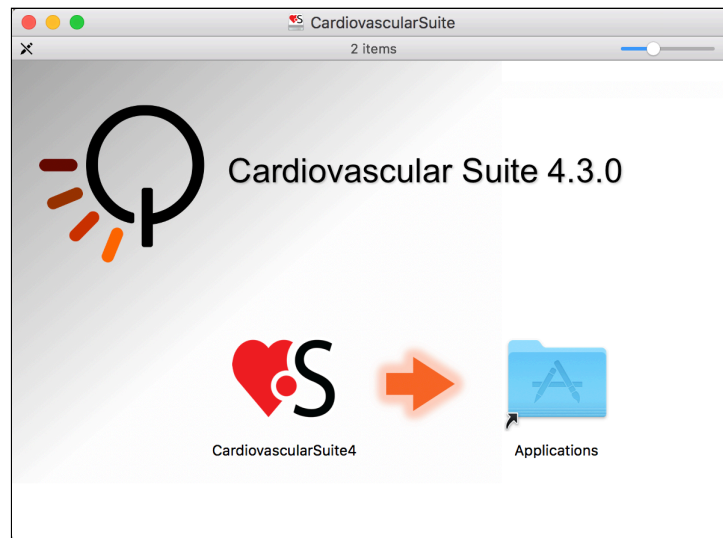


3.3 Microsoft Windows computer


The software installation follows the usual procedure of installing software on Microsoft Windows.

For information or support please contact Quipu support team at support@quipu.eu.


1. Confirm that the installer can make changes to your device .

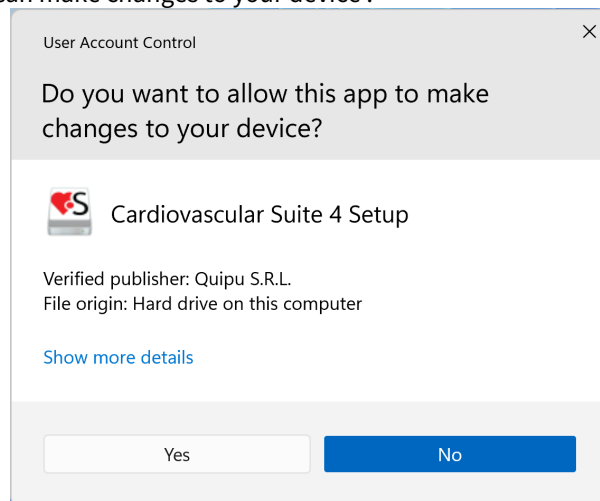


2. Select the language that will be used during the installation.

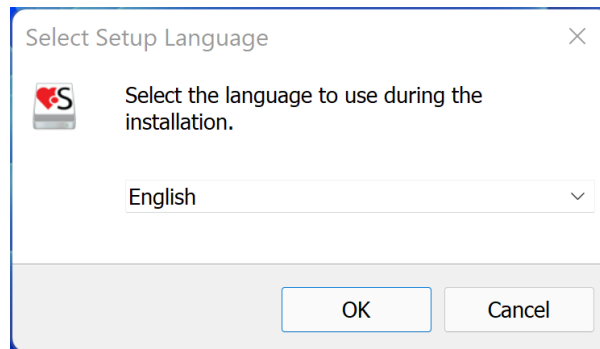


3. Read the License Agreement. If you don't accept the license agreement, please close the Cardiovascular Suite setup. If you accept, click the "Next" button to proceed.

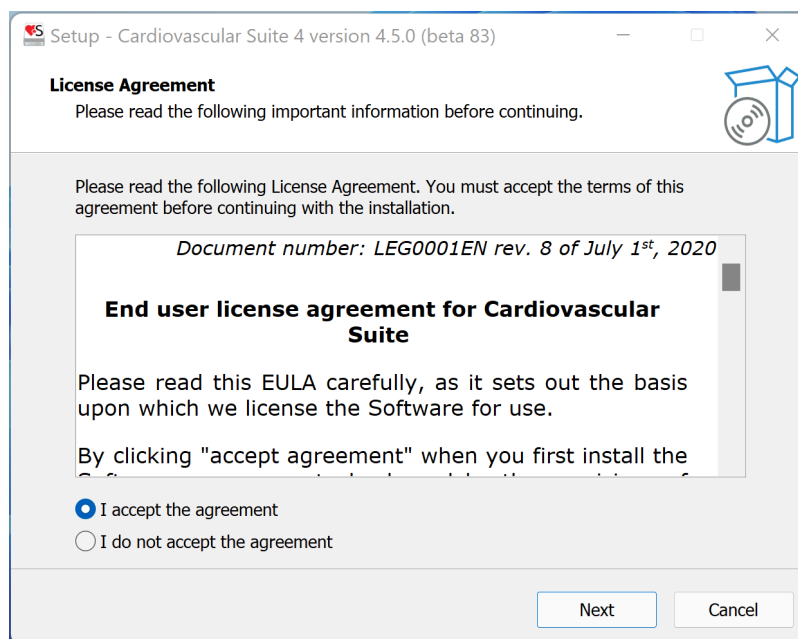


4. Select the installation folder. In most cases, you can use the proposed installation folder. Click the "Next" button to proceed.

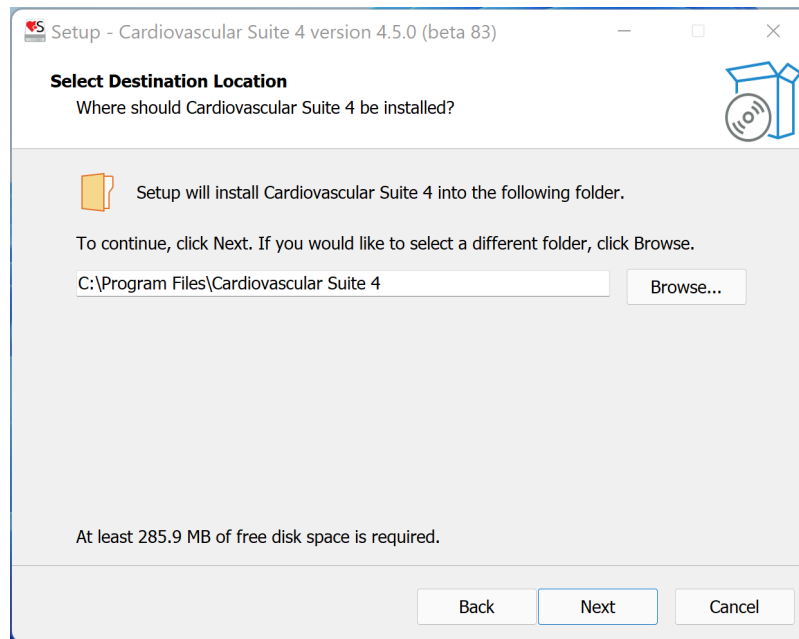


5. Select whether you want to create a Desktop Icon. Click the "Next" button to proceed.

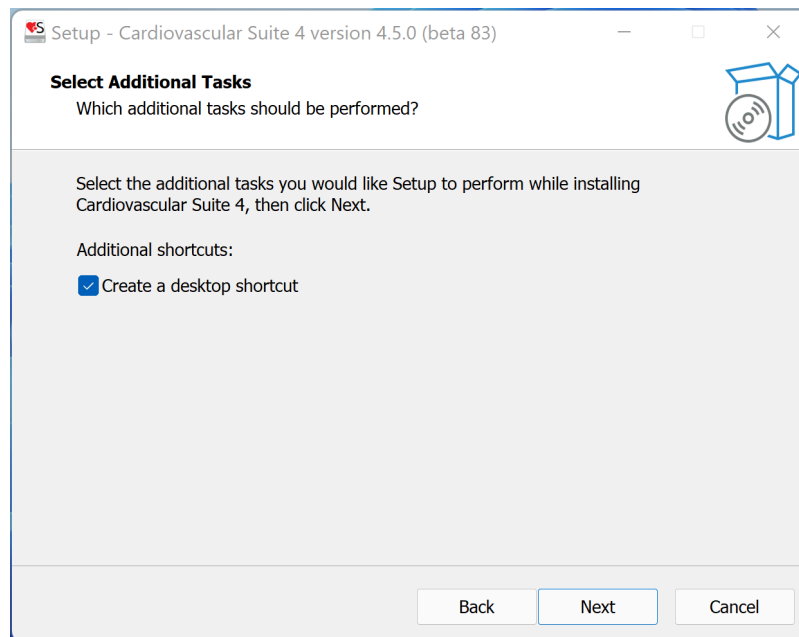

6. Review the installation setting. Click the "Install" button to start installation. Cardiovascular Suite will be installed.

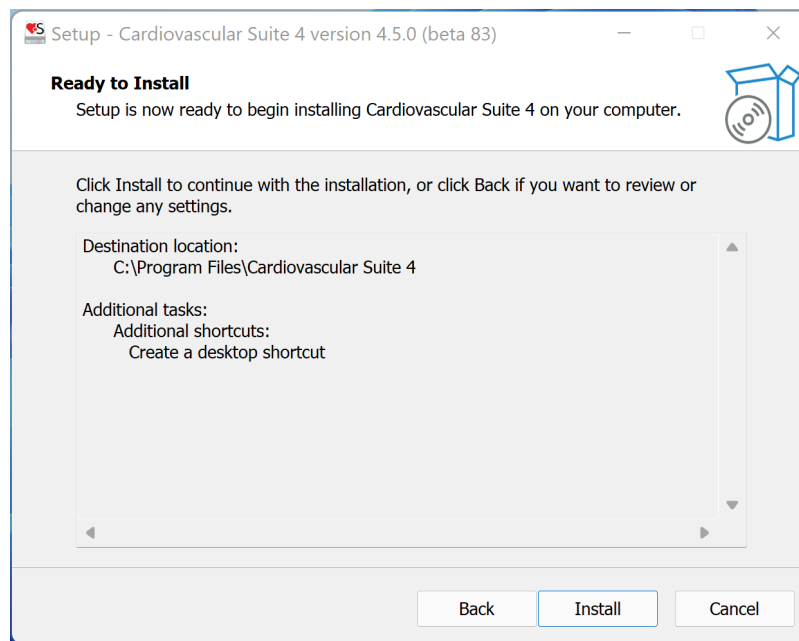


7. When the installation is completed, please click the "Finish" button.

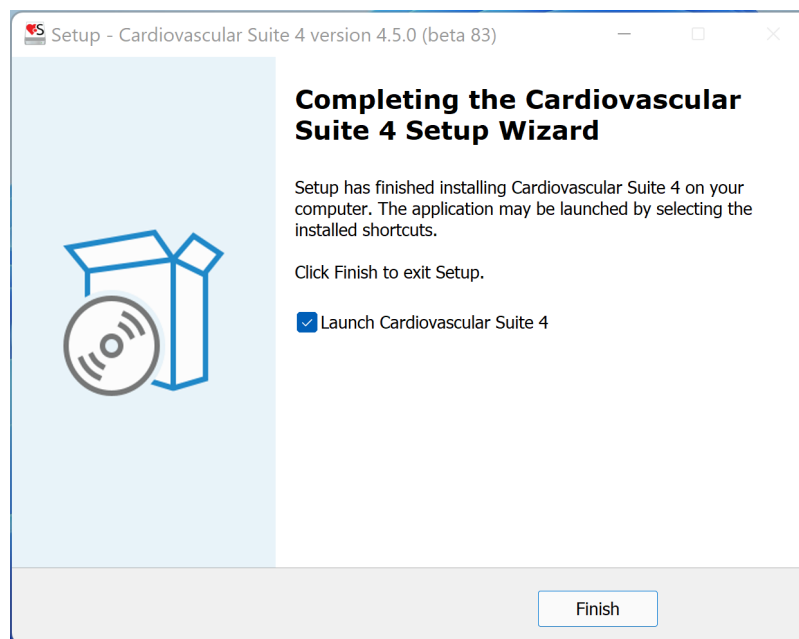

3.4 Archive folder

When Cardiovascular Suite runs the first time, it creates the archive folder, where all the data will be stored. The archive folder is a local folder of the Windows/macOS user. This means that if Cardiovascular Suite is used by different Windows/macOS users on the same computer, each Windows/macOS user will have his/her own archive.

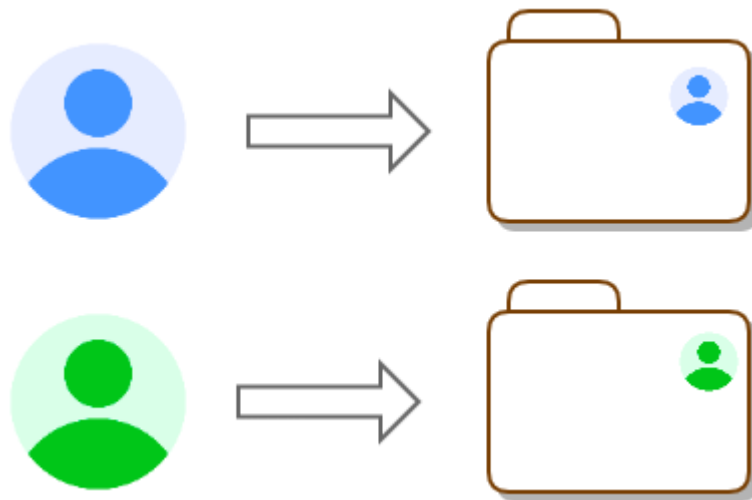

The archive folder is located at the following address:

- Apple Computers: ~/Library/Application Support/CardiovascularSuite4
- Windows Computers: %AppData%\..\Local\cardiovascular_suite4

⚠ CAUTION: It is recommended to perform regular backups of the system. The non-operation of the backup could result in permanent data loss.

3.5 Moving to a new computer

The steps necessary to migrate Cardiovascular Suite to a new computer are:

1. Copy the archive folder(s)
2. Install Cardiovascular Suite
3. Migrate the license

3.5.1 Copying the archive folders

Copy the archive folder from the old computer to the new computer. The archive folder must be placed in the local folder of the Windows/macOS user who will use the software. If the old computer was used by more than one Windows/macOS users, you may have more than one archive folder to be copied in the new computer.

The archive folder is located at the following address:

- Apple Computers: ~/Library/Application Support/CardiovascularSuite4
- Windows Computers: %AppData%\..\Local\cardiovascular_suite4

3.5.2 Installing Cardiovascular Suite

Install Cardiovascular Suite on the new computer. The last version of the software installer can be downloaded from the following links:

- Windows Computers: <http://www.quipu.eu/download/CardiovascularSuiteWin.php>
- Apple Computers: <http://www.quipu.eu/download/CardiovascularSuiteMac.php>

For previous versions of the software, please contact our support team at: support@quipu.eu

3.5.3 Migrating the license

If you have a Quipu License Key, plug it in the new computer. The license may not work because still locked to the old computer. In that case, an error message will be displayed when you run Cardiovascular Suite. Please contact the Quipu support team (support@quipu.eu) for migrating your license to the new computer.

3.6 Extraordinary maintenance

There are no updates of parts of the software. In case of correction of "bugs", the user is alerted via e-mail and the software can be re-installed in the usual manner described in the [Installation](#) instructions.

The last version of the software installer can be downloaded from the following links:


- Windows Computers: <http://www.quipu.eu/download/CardiovascularSuiteWin.php>
- Apple Computers: <http://www.quipu.eu/download/CardiovascularSuiteMac.php>

For previous versions of the software, please contact our support team at: support@quipu.eu

The archive of the software is not deleted when uninstalling/installing the software. The backup of the archive folder is recommended before uninstalling/installing the software. If you want to delete all the data previously created with Cardiovascular Suite, you must delete the archive folder.

The archive folder is located at the following address:

- Apple Computers: ~/Library/Application Support/CardiovascularSuite4
- Windows Computers: %AppData%\..\Local\cardiovascular_suite4

 **CAUTION: the backup of the archive folder is recommended before uninstalling/installing the software.**

3.7 Decommissioning and disposal

The user can safely decommission and dispose the Cardiovascular Suite and the license key.

In particular, the software can be uninstalled following the usual procedure of uninstalling software on Apple computers or Windows computer. The uninstalling procedure does not delete the archive of the software. These data should be removed manually by deleting the archive folder that is located at the following address:

- Apple Computers: ~/Library/Application Support/CardiovascularSuite4
- Windows Computers: %AppData%\..\Local\cardiovascular_suite4



The license key can be disposed according to the local regulation regarding the waste management.

⚠ CAUTION: the data produced by Cardiovascular Suite are not deleted during the software uninstall procedure. They should be removed manually by deleting the archive folder.

4 License

Cardiovascular Suite is licensed under the [EULA](#).

Cardiovascular Suite has independent licenses for FMD Studio and Carotid Studio. You can choose between two types of license:

- **Perpetual License:** it is a license that never expires. With the Perpetual License you are entitled to run all the minor updates of the application. For example, if you have a perpetual license for FMD Studio ver. 3, you will be entitled to run FMD Studio ver. 4.0, 4.1, 4.2 and so on, but you will not be entitled to run FMD Studio ver. 5.0
- **Time License:** it is a time limited license. With this license, you are entitled to run any version of the application within the expiry day. After the expiry date, it is no longer possible to run the application or modify the stored data.

Cardiovascular Suite is licensed by the Quipu License Key, which is a USB dongle key.



Quipu License Key

When you receive the Quipu License Key, it will contain a not activated license. Please follow the instruction for [Activating a license](#).

Once activated, your license will be stored inside your Quipu License Key.

⚠ CAUTION : The Quipu License Key contains your license. Store it in a safe place in order to avoid loss and / or theft.

The Quipu License Key must be plugged into the computer where the software is running. If you unplug the Quipu License Key while Cardiovascular Suite is running, the software will stop working.


Your license will work only on the computer where the Quipu License Key is used for the first time (i.e. it will be locked to this computer). If you want to replace your computer, please contact the Quipu support team (support@quipu.eu) for instructions on how to move your license to the new computer. You are allowed to move your license in a new computer three times in a year.

⚠ CAUTION : The Quipu License Key will work only on the computer where it is used for the first time.


4.1 Activating a license

Plug the Quipu License Key into your computer and run Cardiovascular Suite.


The following form is shown. Please enter your data to register and activate the license (all fields are mandatory). Then, click on the OK button.

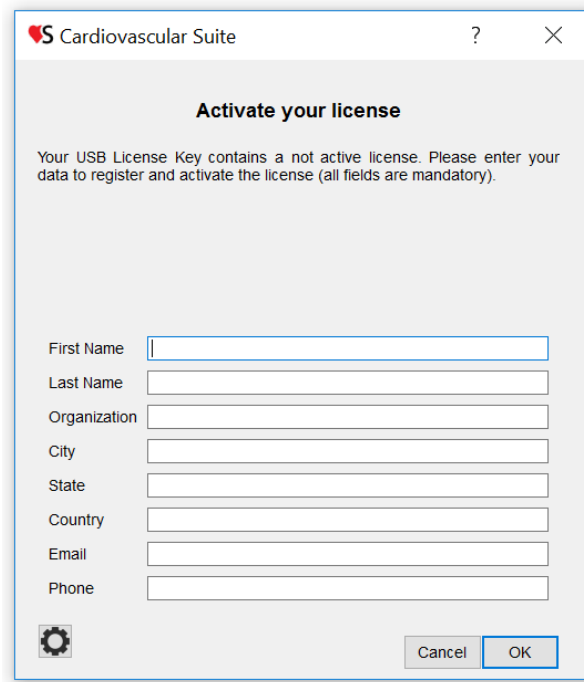


After a few seconds, a confirmation message will appear. Click on the OK button and Cardiovascular Suite will start automatically.

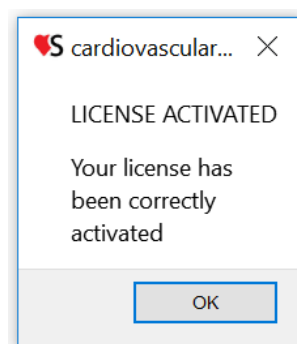

If activation failed, proceed with offline activation by clicking the Offline button.

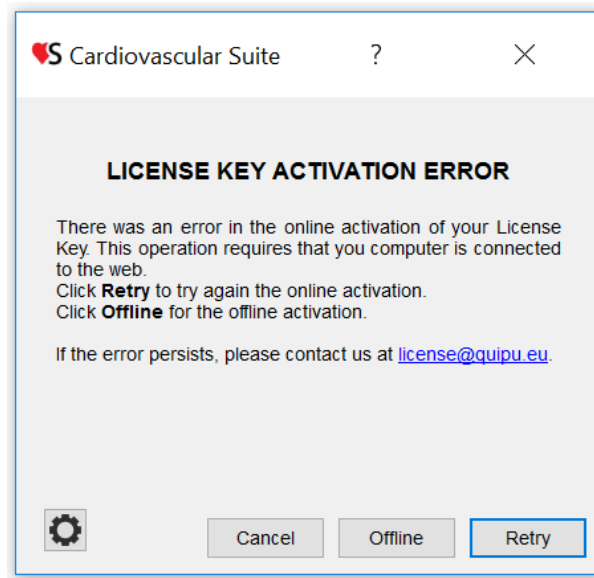


The following message will be shown:

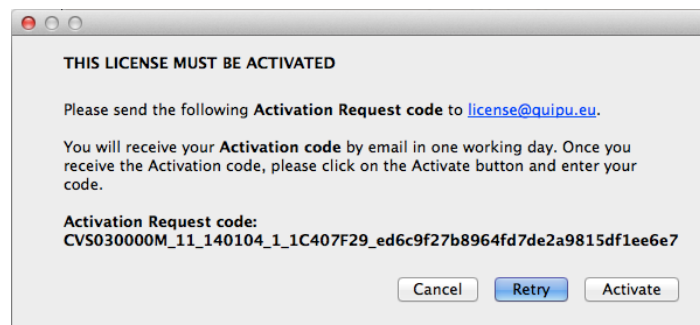

Click on the license@quipu.eu; if you have a mail application on your computer, it will generate a pre-compiled email with your data (Name, Organization, City, Country) and the **Activation request code** that is displayed on the message. Otherwise, please send an email to license@quipu.eu containing your data (Name, Organization, City, Country) and the **Activation request code** that is displayed on the message.


Within a working day, you will receive an email with the **Activation Code**.

You can now click on the Activate button. The following message is shown:

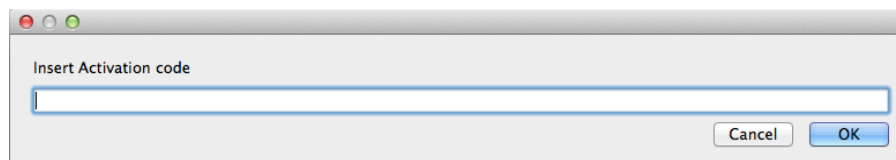




Enter your Activation code and click OK. A confirmation message is shown.

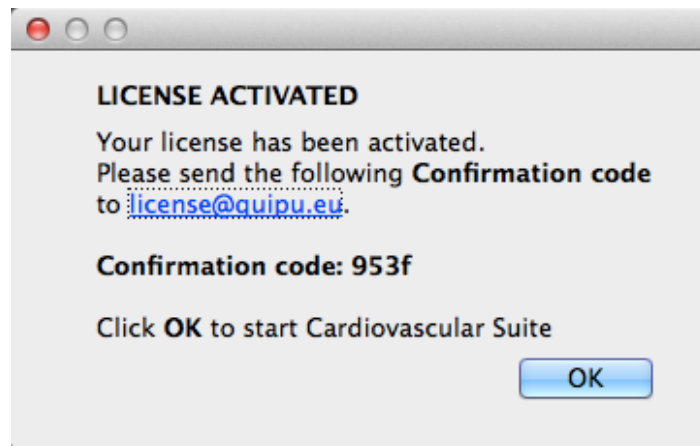

Please send the Confirmation Code to Quipu by email, then click OK to start Cardiovascular Suite.

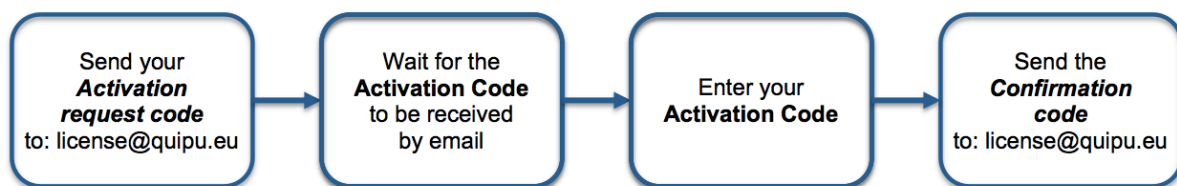

4.2 Evaluation license


You can evaluate Cardiovascular Suite by a 14 days evaluation license.

With this license, you are entitled to use Cardiovascular Suite **only for EVALUATION PURPOSES**. If you wish to use the software for any other purpose, you must purchase a commercial license. If you do not purchase a commercial license, at the end of the 14 days your content will no longer be available to you.


You cannot use/publish/distribute data generated by the Cardiovascular Suite in the evaluation period unless you purchase a commercial license.

 **Please, note that an Internet connection is needed to obtain and use the Evaluation License**

After downloading and installing the software, run Cardiovascular Suite. The following message is displayed:

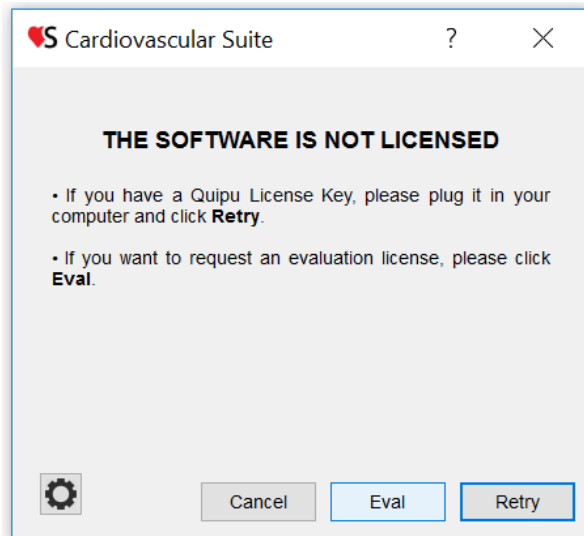


Click on the Eval button to request a fully functional 14-days Evaluation License. The following form is shown:

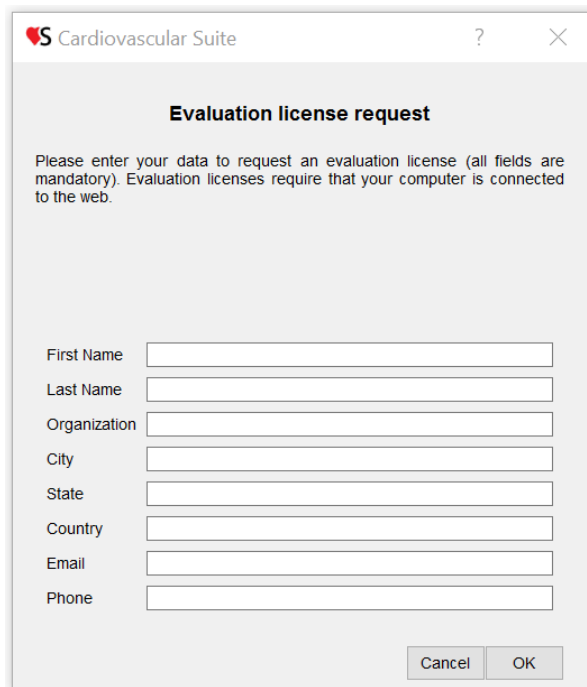

The screenshot shows a dialog box titled "S Cardiovascular Suite" with a red heart icon and a question mark. The main text reads "Evaluation license request". Below this, there is a paragraph: "Please enter your data to request an evaluation license (all fields are mandatory). Evaluation licenses require that your computer is connected to the web." Below the paragraph, there are eight input fields: "First Name", "Last Name", "Organization", "City", "State", "Country", "Email", and "Phone". At the bottom right, there are "Cancel" and "OK" buttons.

Please, enter your data to request an Evaluation License (all fields are mandatory). Then, click on the OK button. Please wait and after a few second the following confirmation message will be shown:

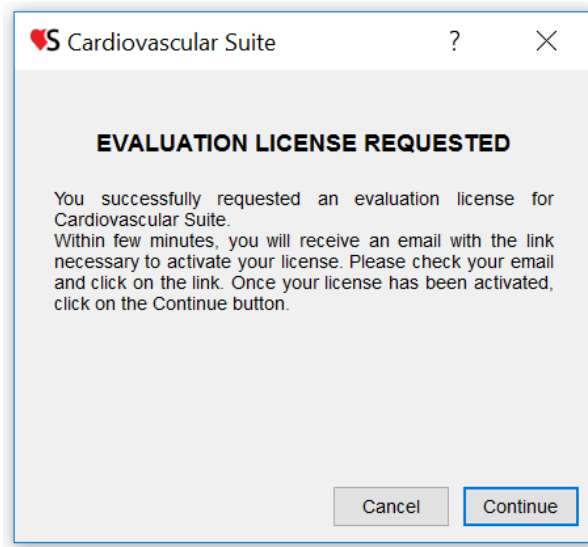

Within few minutes, you will receive an email with the **Activation link**.



Thu 06/07/2017 16:28

Quipu <license@quipu.eu>


Cardiovascular Suite evaluation license activation

Dear customer,
your Evaluation Licence for Cardiovascular Suite has been created.
Click on the following link to activate your evaluation licence:
http://server.quipu.eu/~quipu_server/licensemanager/evalLicenseActivation/7709965C

Thank you for choosing Cardiovascular Suite.

Best regards
The Quipu Team
license@quipu.eu

Click on the **Activation link**. Your web browser will open the following web page and your license will be activated:

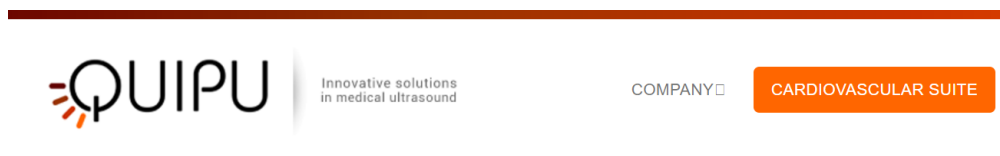


Your license has been activated correctly. You can now evaluate Cardiovascular Suite

If you still have Cardiovascular Suite open with the "Evaluation License Requested" message, please click on the Continue button. Otherwise run again Cardiovascular Suite. Now, the software starts and the [Login](#) window is displayed.

If the Evaluation License Request failed or errors occurred, please contact our technical support by mail or Skype message (support@quipu.eu)

4.3 License manager

The license managers shows the status of your license and can be used to make updates to the license.

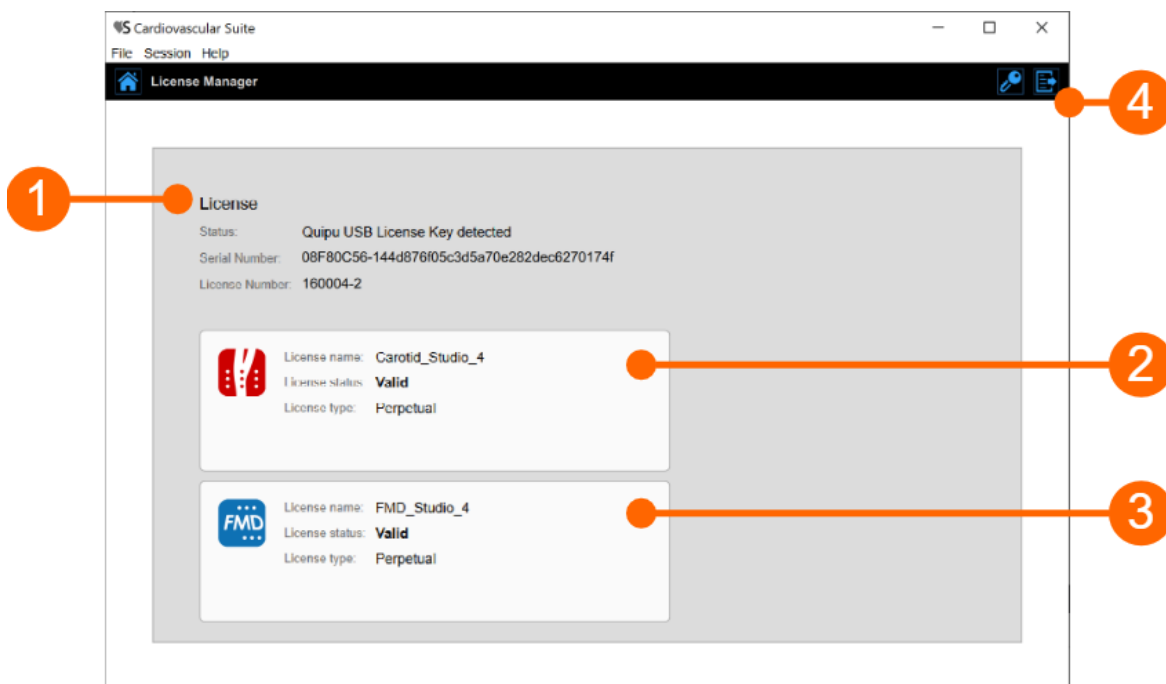

The section **(1)** shows some "general" license data:


Status: shows whether a USB License Key or a temporary License Key has been detected.

Serial Number: shows the serial number of Cardiovascular Suite.



License Number: shows the number of your License Key.

In the white frames **(2)** and **(3)** the data of the applications licenses are shown. Here you can see if your license is Valid or Not Valid, if it is Perpetual, Time or Evaluation and the expiry date (for time and evaluation only).

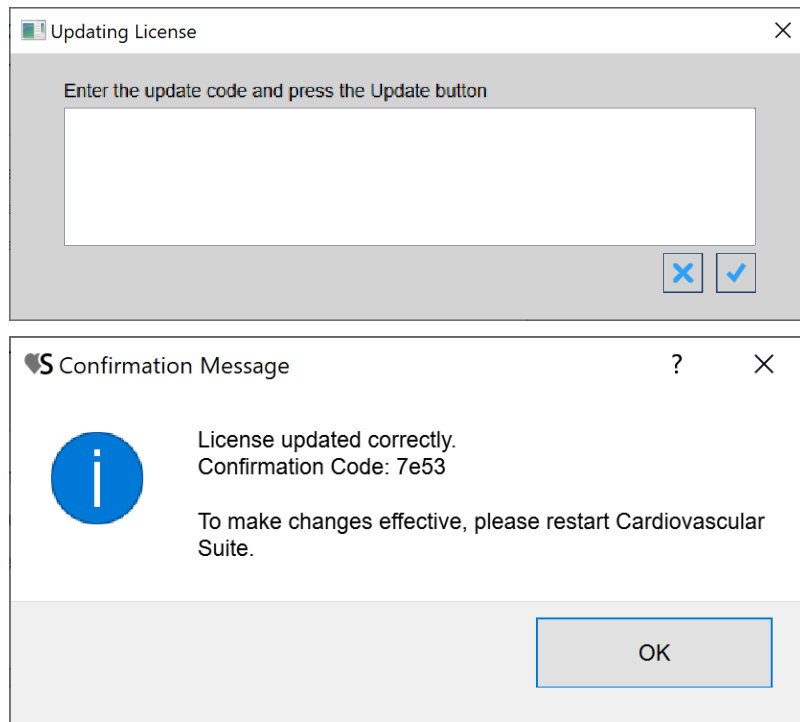
The buttons **(4)** can be used to enter the code that updates your license (Update Code) and to save your license data in a file that can be read by the Quipu support team. For more information, please contact support@quipu.eu



Update a license

- Click on the Update License  button.
- Enter the Update Code provided by Quipu.
- Confirm with the Update  button.
- A confirmation message will show the Confirmation Code. You must restart Cardiovascular Suite to make changes effective.

Export license data

Click on the Export License Data  button to export the data of your license in a file that can be read by the Quipu support team. This can be useful when you encounter a problem with your license and you need support.

5 Image and video sources


The software processes video images coming from a medical ultrasound equipment. It can work:

- **offline** by processing video clips or single images previously recorded on the ultrasound imaging device. See [Using image or video clip for offline analysis](#).
- in **real-time** by processing the video output of the ultrasound imaging system. See [Connecting your computer to the ultrasound system](#).

5.1 Using image or video clip for offline analysis

Video clips or single images recorded on the ultrasound imaging device can be moved on the computer using a digital medium (flash pen drive, hard disk, CD ROM). Video files can be in DICOM 3 or in all the most common video formats (AVI, MOV, MP4, ..). The images can be in all the most common image formats (JPG, PNG, TIFF, GIF, BMP, ..).


For more information on supported video formats, please contact support@quipu.eu

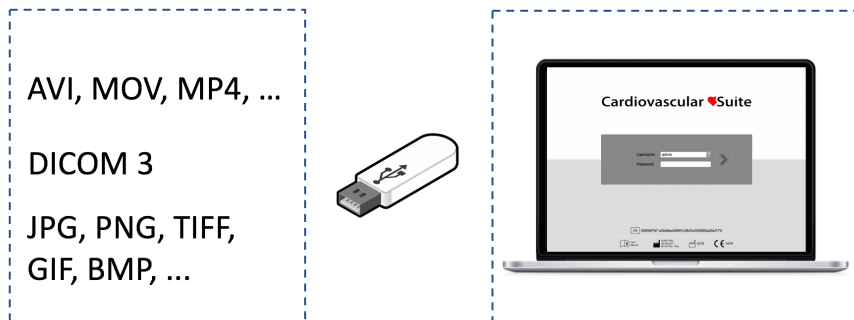

CAUTION: The B-mode window in the image must have a minimal resolution of 6 pixels/mm. If present, the size of the PWD window in the image must be at least 200x100 pixels.


5.2 Video and image player

The video and the images are displayed in a player like in the following figure.

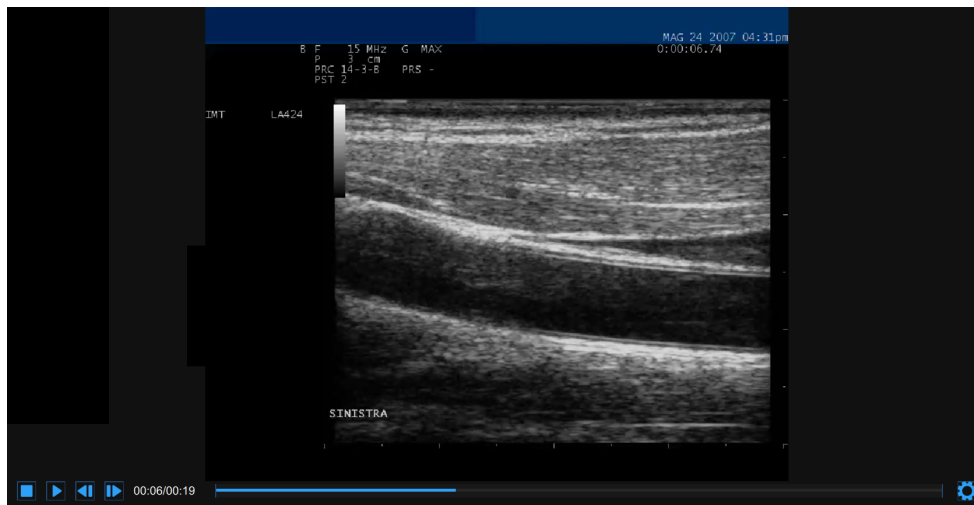







At the bottom of the video and image player, a control bar is present. The control bar contains different controls if the source is online or offline, and if a video or an image is played.

Control bar - online

The control bar contains the elapsed time and the Setting  button.




Control bar - offline video

The control bar contains controls to manage the playback of a movie (Stop , Play  /Pause , Step backward  and Step forward  buttons), the current and total time, and the Setting  button.




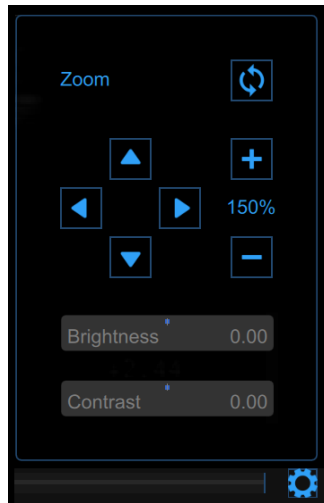
Control bar - offline image



The control bar contains the Setting  button.



5.2.1 Video and image settings

Click on the Setting  button on the right of the video control bar. The Zoom controls and the Brightness and Contrast sliders will be shown.



Click the Zoom in  / Zoom out  buttons to zoom in and out the image.

Click the Move up  / Move down  / Move Left  / Move right  button to move up / down / left / right the zoomed image.

Click the Reset zoom button  to reset the image zoom.

Drag the brightness slider  to adjust the brightness of the image.

Drag the contrast slider  to adjust the contrast of the image.


5.3 Connecting your computer to the ultrasound system

You need a video capture device to connect the computer with the ultrasound system and perform real-time analysis. Quipu recommends two USB devices: the [Epiphan AV.io HD](#) or the [Magewell USB Capture AIO](#).

If your ultrasound machine has a [VGA/DVI/HDMI output](#) (see next figure for reference), you can directly connect your ultrasound machine to the computer by using either the [Epiphan AV.io HD](#) or the [Magewell USB Capture AIO](#) video capture device. ([See more...](#))



VGA

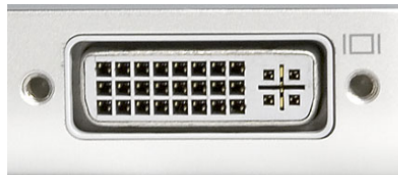

DVI



HDMI

If your ultrasound machine has a "legacy" video standard ([S-Video](#) or [C-Video](#)) output (see next figure for reference), you can directly connect your ultrasound machine to the computer by using the [Magewell USB Capture AIO](#). If you want to use the [Epiphan AV.io HD](#), you must first convert the video output to VGA, and then to acquire the VGA by the [Epiphan AV.io HD](#). For the first video conversion, you can use any high-quality S-Video to VGA or C-Video to VGA


converter. We suggest using the [StarTech Video to VGA Converter v4.3](#) ([See more ..](#))



S-Video



C-Video (RCA)



C-Video (BNC)

	Epiphan AV.io HD	Magewell USB Capture AIO
VGA	Directly supported	Directly supported
DVI	Directly supported	Directly supported
HDMI	Directly supported	Directly supported
S-Video	Conversion to VGA is required	Directly supported
C-Video	Conversion to VGA is required	Directly supported

NOTE: Please, verify with the ultrasound machine technician that the video output of your ultrasound machine is active.

For information on the availability and the standard of the video output, please contact the manufacturer of the ultrasound system.

For additional technical information on how to connect the computer to the ultrasound apparatus and on the compatible video standards, please contact us at support@quipu.eu


CAUTION: The B-mode window in the video must have a minimal resolution of 6 pixels/mm. If present, the size of the PWD window in the image must be at least 200x100 pixels.

CAUTION: The ultrasound scanner must be in accordance with the European Medical Device Directive 93/42/EEC or cleared / registered / licensed by the appropriate regulatory authority.

⚠ CAUTION: If the video converter is used with an AC/DC power adapter, it must be a medical grade power adapter according to IEC 60601-1, current edition.

5.3.1 Using VGA/DVI/HDMI output

You can directly connect your ultrasound machine to the computer by using either the [Epiphan AV.io HD](#) or the [Magewell USB Capture AIO](#) video capture device.

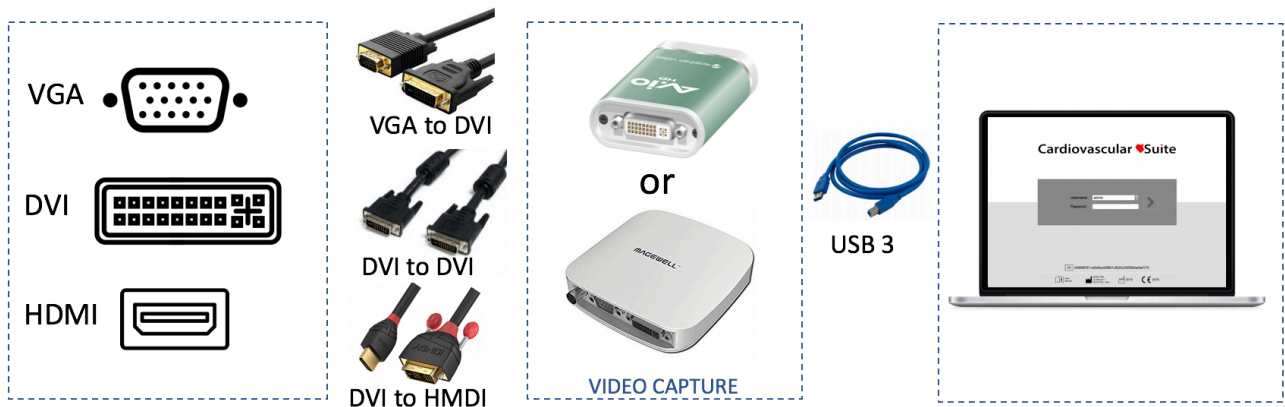

Detail of the connections based on the output video format:

- **VGA video output:** use a VGA-to-DVI cable to connect your ultrasound machine to the Epiphan AV.io HD or the Magewell USB Capture AIO; then use the USB 3.0 cable to connect the video capture device to your computer.
- **DVI video output:** use a DVI cable to connect your machine to the Epiphan AV.io HD or the Magewell USB Capture AIO; then use the USB 3.0 cable for connecting the video capture device to your computer.
- **HDMI video output:** use an HDMI to DVI cable to connect your ultrasound machine to the Epiphan AV.io HD or the Magewell USB Capture AIO; then use the USB 3.0 cable to connect the video capture device to your computer.

See more about the [Epiphan AV.io HD](#) or the [Magewell USB Capture AIO](#).

5.3.2 Using "legacy" video standard output

5.3.2.1 Magewell USB Capture AIO

You can directly connect your ultrasound machine to the computer by using the [Magewell USB Capture AIO](#) video capture device.




Detail of the connections based on the output video format:

- **S-Video output:** use an S-Video cable to connect your ultrasound machine to the Magewell USB Capture AIO.
- **C-Video (RCA) output:** use an RCA cable to connect your ultrasound machine to the Magewell USB Capture AIO.
- **C-Video (BNC) output:** use a BNC-to-RCA adapter and then an RCA cable to connect your ultrasound machine to the Magewell USB Capture AIO.

Use the USB 3.0 cable to connect the video capture device to your computer. See more about [Magewell USB Capture AIO](#).

5.3.2.2 Epiphan Av.io HD

You must first convert the video output to VGA by the [StarTech Video to VGA Converter](#), and then to acquire the VGA by the [Epiphan AV.io HD](#).

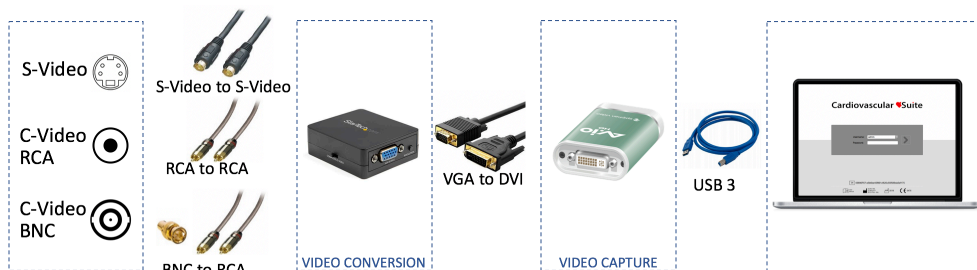

Detail of the connections based on the output video format:

1. First, connect your apparatus video output to the [StarTech Video to VGA Converter](#).
 - **S-Video output:** use an S-Video cable to connect your ultrasound machine to the StarTech Video to VGA Converter.
 - **C-Video (RCA) output:** use an RCA cable to connect your ultrasound machine to the StarTech Video to VGA Converter.
 - **C-Video (BNC) output:** use a BNC-to-RCA adapter and then an RCA cable to connect your ultrasound machine to the StarTech Video to VGA Converter.
2. Once you have connected your apparatus to the StarTech Video to VGA Converter, you have to connect it to your computer by the [Epiphan AV.io HD](#). You have to use the DVI-to-VGA cable to connect the Video Converter to the Epiphan AV.io HD. Then, use the USB 3.0 cable to connect the video capture device to your computer.

See more about the [Epiphan AV.io HD](#).

See more about the [About StarTech Video to VGA Converter](#).

5.3.3 About Magewell USB Capture AIO

The USB Capture AIO is a USB2.0/USB3.0 video capture device from Nanjing Magewell Electronics Co., Ltd, China.

The device can be used to connect your computer to DVI, VGA, HDMI, S-Video and Composite video outputs coming from the ultrasound system. See [Connecting your computer to the ultrasound system](#) for more details.

There's no software to install to use USB Capture AIO; simply connect the cables and go. It works on Microsoft Windows computers and Apple Mac OS X computers.



Once you have connected your ultrasound apparatus to the USB Capture AIO, connect your computer to the video converter via the USB cable. The red LED (PWR) shows that the device is powered on. The green LED (ACT) shows the status of the device.

GREEN LED (ACT)	STATUS
Pulsing slowly	Idle
ON	Input signal connected
OFF	Input signal unconnected
Double blinks	Memory failed or FPGA configuration failed

The USB Capture AIO supports resolution up to 2048x2160. Performance may be limited by your computer features.

The Magewell USB Capture AIO supports both USB 3.0 and USB 2.0.

⚠ CAUTION: the video converter must be connected directly to a USB port on your computer. Do not use hubs or the USB socket on the external keyboard. Use USB 3.0 to maximize performances.

⚠ CAUTION: verify that the video output type and resolution of the ultrasound scanner are compatible with this video converter.

5.3.4 About Epiphan AV.io HD

The AV.io HD is a USB2.0/USB3.0 video capture device from Epiphan Systems Inc. Canada.

The device can be used to connect your computer to DVI, VGA or HDMI video outputs coming from the ultrasound system (or coming from a Video Converter if you use "legacy" standard video output). See [Connecting your computer to the ultrasound system](#) for more details.

There's no software to install to use the AV.io HD; simply connect the cables and go. It works on Microsoft Windows computers and Apple Mac OS X computers.



1. Once you have connected your ultrasound apparatus to the AV.io HD, connect your computer to the video converter via the USB cable. The lighting of the **red** LED indicates that the device is initializing.
2. After a few seconds, the LED turns **blue or green** to indicate proper connection between computers and video converter.
3. Connect the video converter to the ultrasound device via the VGA, DVI or HDMI cable.
4. The LED will be **blue or green** until you start capturing a video signal.
5. LED will be **blinking green** or **blinking blue** during the acquisition of a video signal.

LED COLOR	STATUS
OFF	Video converter not connected to the computer
Solid red	AV.io HD initializing
Blinking red	Adjustment to VGA input in progress

Solid green or blue	USB connection active
Blinking green or blue	Video and/or audio transferring successfully

The Epiphan AV.io HD supports resolution from 640x360 up to 1920x1200. Performance may be limited by your computer features.

The Epiphan AV.io HD supports both USB 3.0 and USB 2.0.

CAUTION: the video converter must be connected directly to a USB port on your computer. Do not use hubs or the USB socket on the external keyboard. Use USB 3.0 to maximize performances.

CAUTION: the AV.io HD must be updated with the last firmware from Epiphan System Inc.

CAUTION: verify that the video output type and resolution of the ultrasound scanner are compatible with this video converter.

5.3.5 About StarTech Video to VGA Converter

The Video to VGA Converter from StarTech (Canada) will allow you to convert your S-Video or Composite Video output to a VGA.



	COMPONENT	FUNCTION
--	-----------	----------

1	Video Input Selection Switch	Select the Source Device Video Signal
2	VGA Output Port	Connect a VGA Video Display Device
3	Resolution Selection Button	Select the Output Resolution
4	Power Port	Connect a Power Source
5	Composite Video Input Port	Connect a Composite Video Source Device
6	S-Video Input Port	Connect an S-Video Source Device

5.3.5.1 How to use the StarTech Video to VGA Converter

- Determine if the Ultrasound system has a Composite or S-Video output. Toggle the Video Input Selection Switch **(1)** to match your Ultrasound system video output.
- Connect a Composite Video Cable to the Composite Video Input Port **(5)**, or Connect an S-Video Cable to the S-Video Input Port **(6)**.
- Connect the other end of the Composite Video Cable to the Composite output of the Ultrasound system, or Connect the other end of the S-Video Cable to the S-Video output of the Ultrasound system.
- Connect a VGA Cable to the VGA Output Port on the Video Converter **(2)**.
- Connect the other end of the VGA Cable to the Epiphan AV.io HD.
- Connect the Medical Grade USB Power Adapter to the Power Port **(4)**.
- Select the output resolution by pressing the Resolution Selection Button **(3)** until the desired resolution is met. Each time you press the Resolution Selection Button the new resolution settings will appear on the On Screen Display (OSD) in the upper right-hand corner of the screen. We suggest to use the following resolution: **800x600 P60**.

5.4 How to set up the ultrasound system

Cardiovascular Suite is based on image processing of a B-mode ultrasound scans. The quality of the results can depend on the quality of the ultrasound image supplied to the system.

The ultrasound device must have the following features:

- The ultrasound device must be suitable for vascular imaging and it must be equipped with a **vascular linear probe** with frequency $\geq 5\text{MHz}$ (a range 7-15 MHz is recommended)..
- The ultrasound device must have the **B-mode** imaging mode.
- For the shear-rate measurement, the ultrasound device must have the **Pulsed Wave Doppler** (PWD) mode, and the B-mode and the PWD must be shown and updated simultaneously on the image (Dual mode).
- For offline analysis, the ultrasound device must export in one of the following formats: **AVI, MOV, MP4, DICOM, PNG, JPG, BMP, TIF**. The size of the images must be $\leq 1920 \times 1200$ px.
- For online analysis, the ultrasound device must have a video output in one of the following formats: **S-Video** or **Composite Video** in PAL or NTSC; **VGA, DVI** or **HDMI** with a resolution up to 1920×1200 pixels.
- The B-mode in the image must have **minimal resolution** of 6 pixels/mm. If present, the size of the PWD window in the image must be at least 200×100 pixels.


- The **frame-rate** of the video must be ≥ 17 frames per second.

The general settings of the ultrasound system must be those suggested by the manufacturer of the apparatus. It is important, however, exclude any noise reduction filters that could degrade the performance of the edge detection algorithm. In particular, it is important to exclude any time filters that cause a smoothing effect on the images in motion. These filters may have different designations (the most common name is **persistence**) depending on the model of ultrasound equipment. Please contact the manufacturer of ultrasound apparatus for information on how to exclude this type of filter.

⚠ CAUTION: The ultrasound device must be suitable for vascular imaging and it must be equipped with a vascular linear probe with frequency greater than 5MHz.


⚠ CAUTION: Exclude any noise reduction filter (especially temporal filters).

The artery should be viewed in longitudinal section and should be as horizontal as possible to the image. For Carotid Studio we recommend an image depth of 3-4 cm.

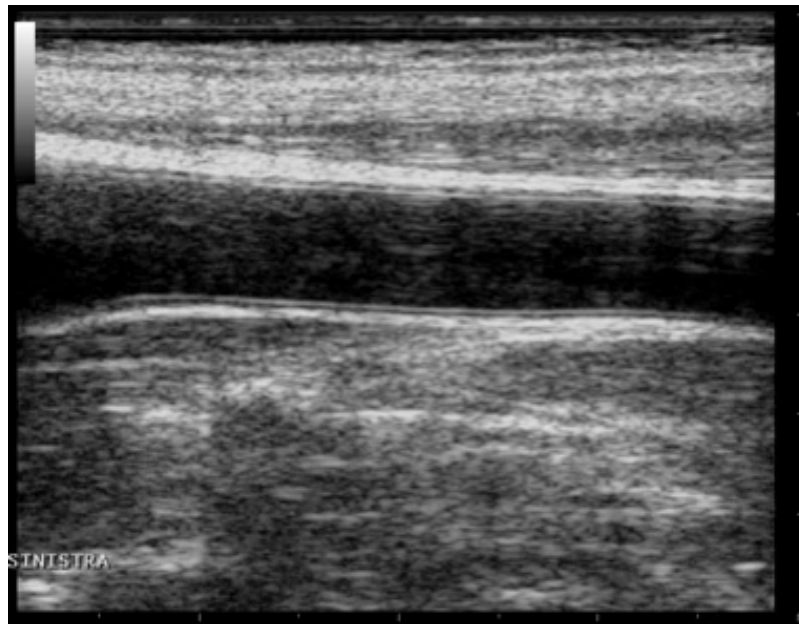

Example of carotid artery image


For FMD Studio we recommend an image depth of 2-3 cm. It is suggested also to choose a projection so that the vein is not visible (this normally appears immediately above the brachial artery). The algorithm for automatic tracking of the edges of the vessel could recognize the edge of the vein instead of the artery.

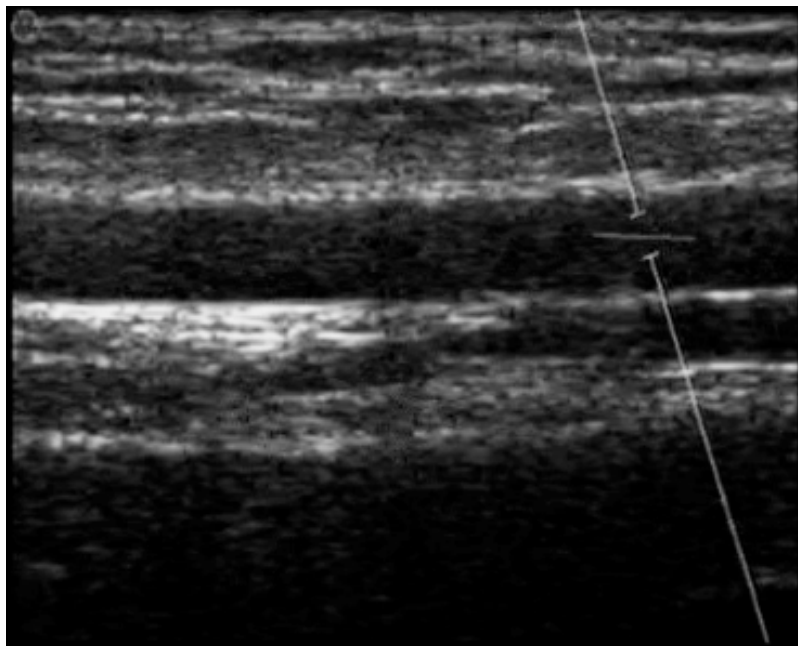

Example of brachial artery image

In addition, for FMD Studio, if you want to obtain both vessel diameter and shear rate, the ultrasound system must be in Duplex mode (simultaneous acquisition of B-mode and Doppler).


The angle between the Doppler beam and the vessel orientation should be ≤ 60 degrees. The sample volume should be as wide as possible but without encompassing the vessel walls and allowing for a slight margin for error in case of movement. Pay attention that the cursor of the doppler sample volume is not into the ROI where the diameter is computed. It is recommended that the sample volume is 5 - 15 mm apart from the ROI.

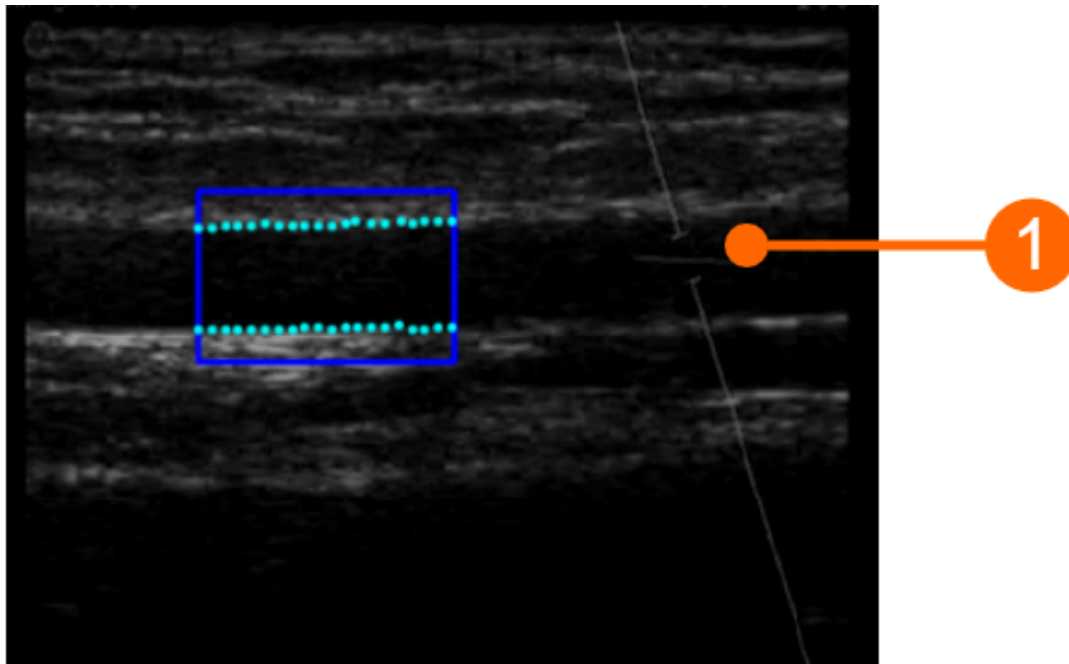

⚠ CAUTION: pay attention that nothing but the ultrasound image is into the ROI. Please note that the processing can be affected by annotations or any other graphical object that is superimposed to the image. In particular, pay attention that the cursor of the doppler sample volume is not into the ROI.

The scale of the Doppler flow profile should be set correctly on the ultrasound system. The vertical scale must be large enough to include the velocity profile during all the examination (in FMD measurements, greater velocity values are in reactive hyperemia). For the horizontal scale, we suggest a value of 3-4 seconds. Please note that the time average is computed over all the extend of the horizontal scale.

The Doppler Flow ROI must cover all the extent of the Doppler flow profile. The zero flow axis **(2)** must be included in the ROI: it will be automatically recognized and plotted in yellow. The vertical axis **(3)** must be external to the ROI. Please also ensure that any annotation **(4)** is outside the ROI since it could affect the flow analysis.

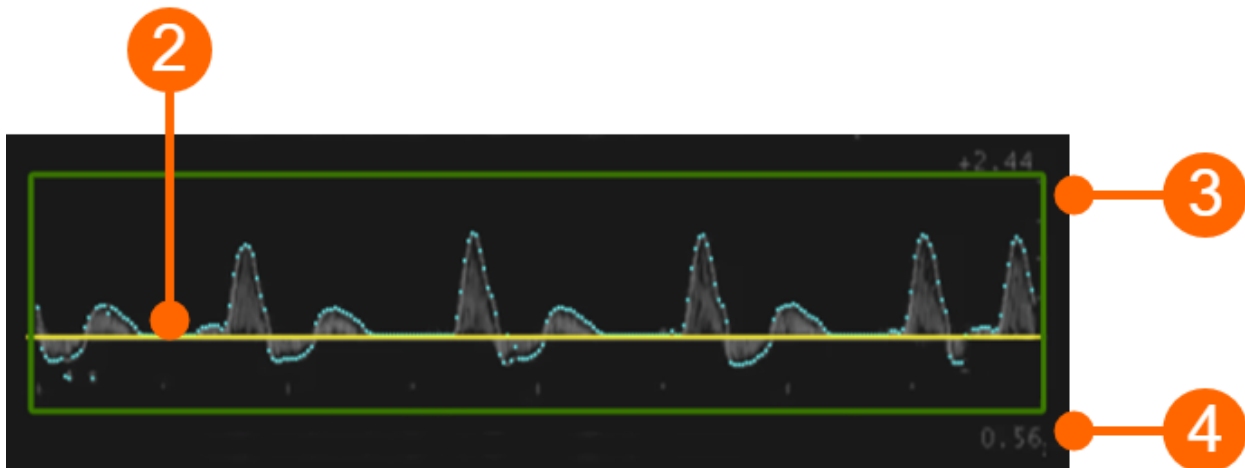

⚠ CAUTION: the processing can be affected by annotations or any other graphical object that is superimposed to the image into the Doppler Flow ROI.

Please remember that the tool for the calculation of the shear rate must be re-calibrated every time you change the size or scale of the Doppler flow profile. This calibration is present in [FMD Studio analysis](#). It is recommended that the size or scale of the Doppler trace will be no longer changed once you have decided how to set up the ultrasound system.

i FMD-Studio precision, expressed as coefficient of variation, is 10% for intra-observer intra-session measurements and 13% for intra-observer inter-session measurements of FMD%. For the Shear Rate measurement, the estimated precision is 2,3%.

Carotid Studio precision expressed as coefficient of variation is 2% for the diameter, 11% for the diameter variation during the cardiac cycle, 6% for IMT for intra-observer intra-session measurements and 3% for the diameter, 12% for the diameter variation during the cardiac cycle, 6% for IMT for intra-observer inter-session measurements. As regards geometric and statistics data the precision of the results expressed as coefficient of variation resulted lower than 10% for each measurement obtained on a single image by the same operator.


6 Login

When you run Cardiovascular Suite, you are asked to login with a Username and Password. Please enter your Username and Password, then click on the Login button to access the software.

✓ When you first run Cardiovascular Suite, the default user account is:

Username: admin

Password: admin

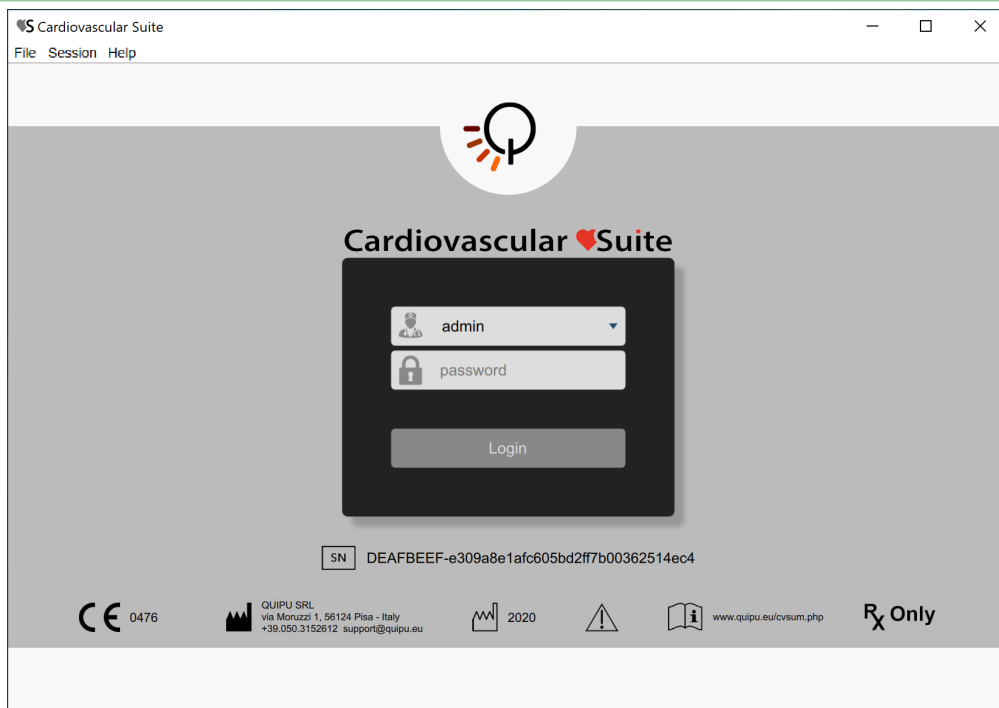

In the lower part of the Login window, the labeling of the device is shown.

In particular, on the right of the **SN** symbol you can find the Serial Number of your software.

Operators

A user account (username and password) is associate to each **operator** of Cardiovascular Suite (an operator is a person who uses Cardiovascular Suite). When the software starts, the operator must login with its user account.


Two classes of operator are available in Cardiovascular Suite:

1. **Users.** They have full access to the software.
2. **Read-only users.** These users can only read the archive and the documents.


An operator is characterized also by a **status** that can be **active** or **disabled**. If an operator has been disabled, he/she cannot access to the software.

It is possible to modify a user account and to add a new one in the [Operators management](#) panel.

7 Home

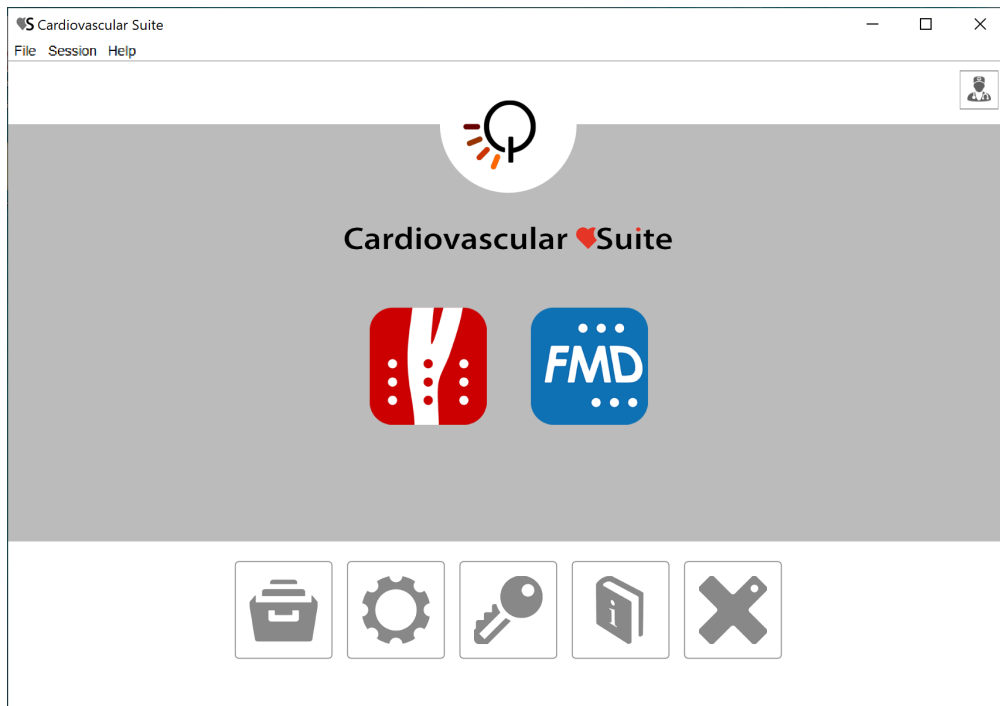

The Home Screen contains the main controls of the software.

The Carotid Studio and the FMD Studio buttons start a new study with [Carotid Studio](#) and [FMD Studio](#) respectively. If a lock icon  is present inside the button, this means that you don't have a valid license for this application.

The buttons in the lower part of the Home Screen are:

- **archive:** opens the [Archive](#) window.
- **settings:** opens the [Settings manager](#) window.
- **license:** opens the [License manager](#) window.
- **manual:** opens this User Manual in an external browser.
- **exit:** quit Cardiovascular Suite.


On the top right of the Home Screen, clicking on the operator icon, you can find the name of the logged user and the logout button.

8 Settings manager

The Settings manager contains the settings of Cardiovascular Suite.

1. [General settings](#)
2. [Carotid Studio settings](#)
3. [FMD Studio settings](#)

8.1 General settings

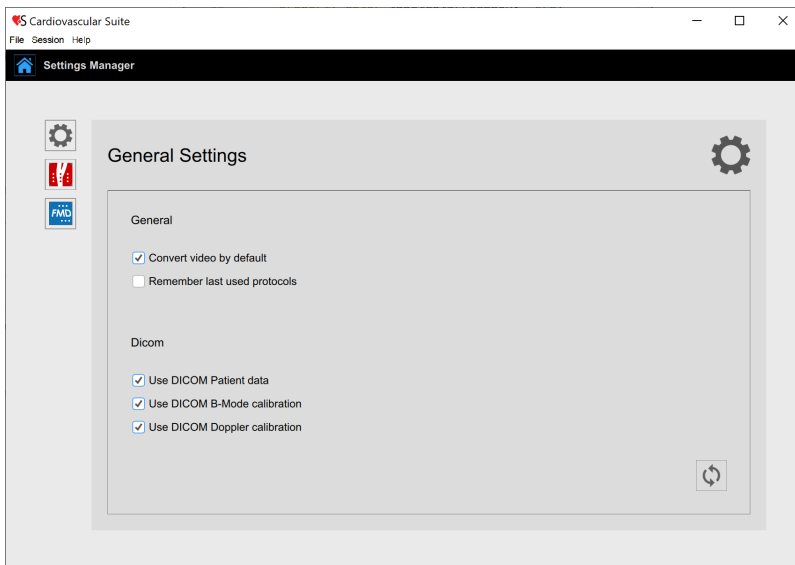


The following settings are available:

General


- **Convert video by default:** if set, when creating a new study, the "Convert video" checkbox is set by default.
- **Remember last used protocol:** if set, when creating a new study, the study will be associated by default with the last used protocols.

Dicom

- **Use DICOM Patient data:** if set, when opening a DICOM file, the patient data are obtained from the file metadata.
- **Use DICOM B-mode calibration:** if set, when opening a DICOM file, B-mode calibration is obtained from the file metadata.
- **Use DICOM Doppler calibration:** if set, when opening a DICOM file, Doppler calibration is obtained from the file metadata.

Every time a change is performed, the software automatically saves it. Click the Restore  button to restore the default options.


8.2 Carotid Studio settings

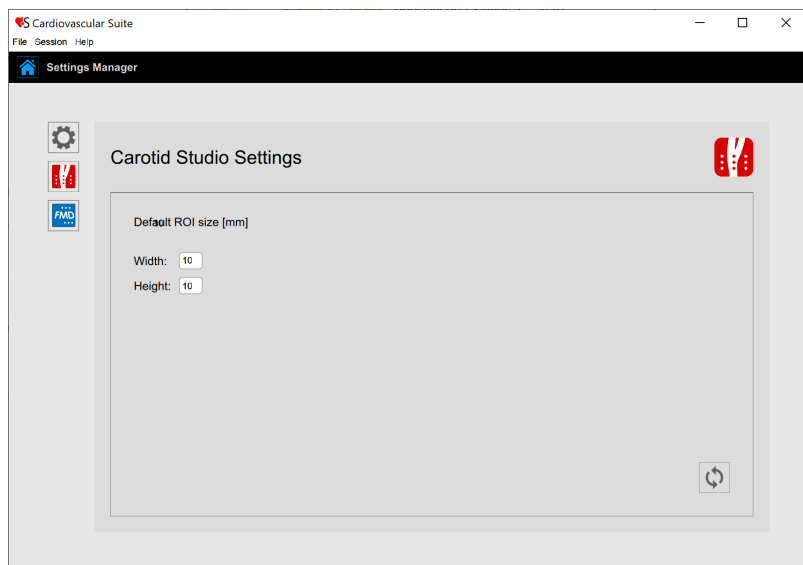


The following settings are available:

Default ROI size

- **Width:** width of the default ROI.
- **Height:** height of the default ROI.

Every time a change is performed, the software automatically saves it. Click the Restore  button to restore the default options.

8.3 FMD Studio settings

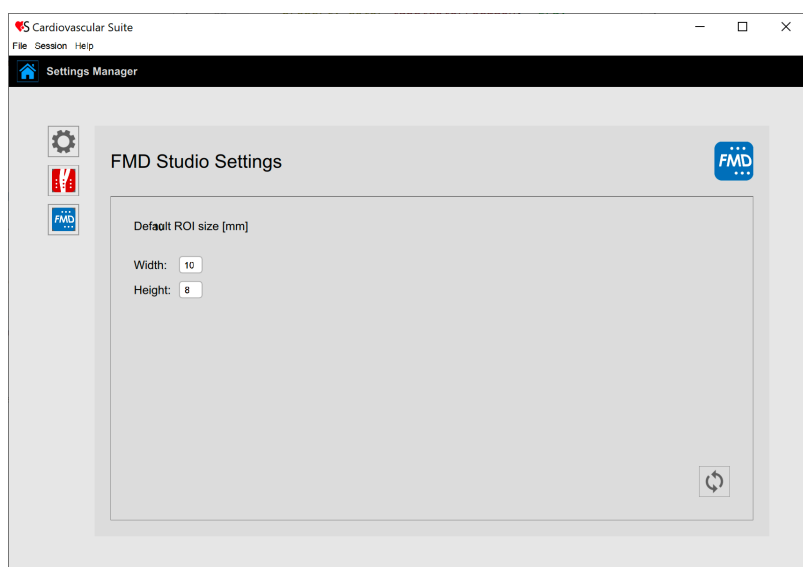




The following settings are available:

Default ROI size

- **Width:** width of the default ROI.
- **Height:** height of the default ROI.


Every time a change is performed, the software automatically saves it. Click the Restore  button to restore the default options.

9 Archive

The Archive is made up by several tabs, that manage:

- the [studies](#) and their [documents](#);
- the [patients](#);
- the [operators](#);
- the [institutes](#);
- the [protocols](#);
- the [tags](#).

9.1 **STUDIES AND DOCUMENTS**

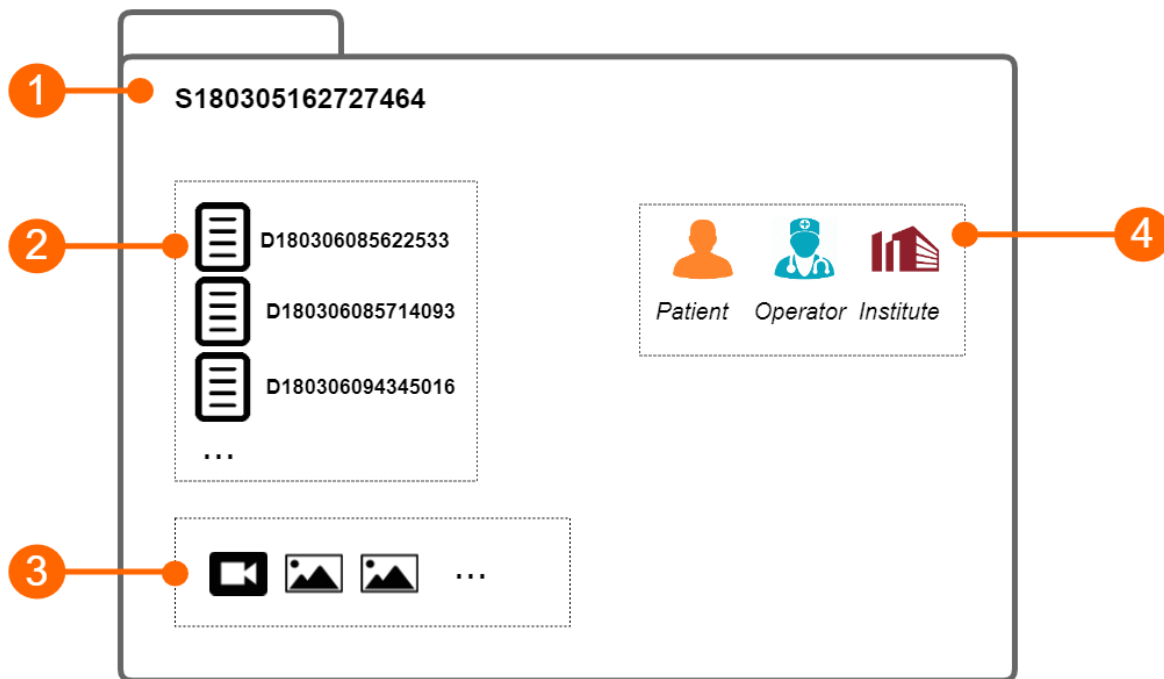

The study (1) contains the results generated by a software application. These results are organized into documents (2). Each document contains the results of the analysis of a video clip or an image. The study instead may contain one or more media files (video clip or images).

Each study has a unique study identification number (study ID), which is a string starting with the letter "S" and followed by 15 numeric digits. Analogously, each document has a unique document identification number (document ID), which is a string starting with the letter "D" and followed by 15 numeric digits.

Each study can be associated with one or more protocols and each document can be associated with one or more tags.

9.2 **PATIENTS**

The patient is the person who undergo the examination.

The archive can contain the following patient data:

- Patient ID
- First name
- Middle name
- Last Name
- Sex (it can be: "Unspecified", "Female" or "Male")
- Birth date (it can be set or "unspecified")
- Address (Street, number, City, ZIP, State/Region, Country)
- Telephone
- E-mail

You can enter no data of the patients. The only mandatory field is the patient ID. If you don't enter patient ID, a random value will be automatically proposed, which is a string starting with the letter "P" and followed by 15 numeric digits.

9.3 **OPERATORS**

The operator is the person who make the examination.

The archive can contain the following operator data:

- First name
- Middle name
- Last Name
- Birth date (it can be set or "unspecified")
- Telephone
- E-mail

You can also set a picture of the operator.

9.4 **INSTITUTES**

The institute is the organization where the examination is performed.

The archive can contain the following institute data:

- Name
- Address (Street, number, City, ZIP, State/Region, Country)
- Telephone
- Fax
- E-mail

You can also set a picture of the institute.

9.5 **PROTOCOLS**

The protocol is a particular experiment or proceeding which a study or more than one may be associated with.

The archive can contain the following protocol data:

- Name
- Description

You can also set a picture of the protocol.

9.6 TAGS

The tag is a particular label which a document, or more than one, may be associated with.

Cardiovascular Suite has two types of tags:

1. **System tags**, which are already defined in the software and are used to specify which documents will be included in the study report.
2. **Custom tags**, which are defined by the user and are used to better identify a document.

Only one system tag can be associated to a document.



Custom tags contain the following tag data:


- Name
- Description

You can also set a picture of the custom tag.

9.7 Studies management

In the Studies and Documents panel, it is possible to manage studies and documents.

This panel is made up by a search field **(1)**, the filter management panel **(2)**, the control buttons **(3)** and a table **(4)** for showing the study list (or the document list), depending on the selected tab ( Studies or  Documents) from the control buttons.

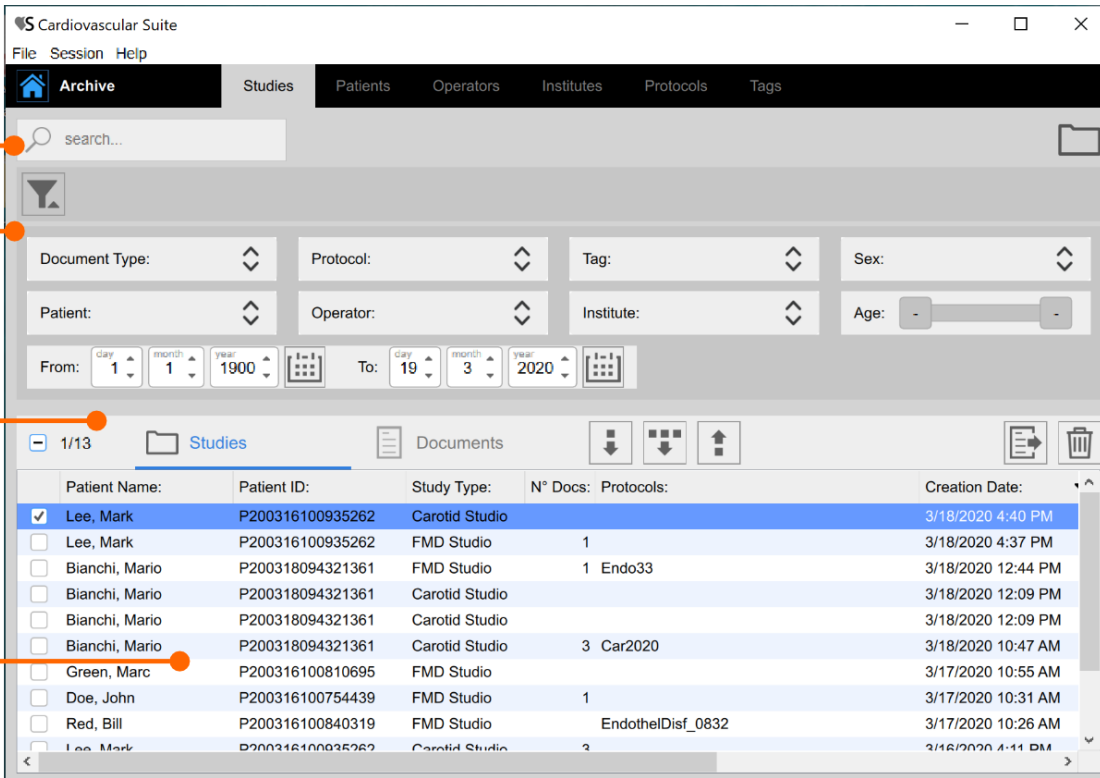


The screenshot shows the 'Cardiovascular Suite' application window. The 'Studies' tab is selected in the top navigation bar. The interface includes a search field (1), a filter management panel (2) with various dropdowns and date pickers, and control buttons (3) for switching between 'Studies' and 'Documents' views. The table (4) displays a list of studies with columns for Patient Name, Patient ID, Study Type, N° Docs, Protocols, and Creation Date.

	Patient Name:	Patient ID:	Study Type:	N° Docs:	Protocols:	Creation Date:
<input checked="" type="checkbox"/>	Lee, Mark	P200316100935262	Carotid Studio			3/18/2020 4:40 PM
<input type="checkbox"/>	Lee, Mark	P200316100935262	FMD Studio	1		3/18/2020 4:37 PM
<input type="checkbox"/>	Bianchi, Mario	P200318094321361	FMD Studio	1	Endo33	3/18/2020 12:44 PM
<input type="checkbox"/>	Bianchi, Mario	P200318094321361	Carotid Studio			3/18/2020 12:09 PM
<input type="checkbox"/>	Bianchi, Mario	P200318094321361	Carotid Studio			3/18/2020 12:09 PM
<input type="checkbox"/>	Bianchi, Mario	P200318094321361	Carotid Studio	3	Car2020	3/18/2020 10:47 AM
<input type="checkbox"/>	Green, Marc	P200316100810695	FMD Studio			3/17/2020 10:55 AM
<input type="checkbox"/>	Doe, John	P200316100754439	FMD Studio	1		3/17/2020 10:31 AM
<input type="checkbox"/>	Red, Bill	P200316100840319	FMD Studio		EndothelDisf_0832	3/17/2020 10:26 AM
<input type="checkbox"/>	Lee, Mark	P200316100935262	Carotid Studio	3		3/16/2020 4:11 PM


9.7.1 Searching and filtering


It is possible to perform a textual search in the Studies or Documents table thanks to the search field on the top **(1)**.

The filter management panel **(2)** allows the possibility to add and remove filters. By clicking on the  icon, the following filters can be added:


- Document type
- Patient
- Operator
- Institute
- Patient Sex
- Patient Age
- Patient Birthdate
- Document Tag
- Study Protocol


In addition, it is possible to filter the studies by patient, operator, and institute by going to their panels and double clicking on one of them.

Once the filter panel is visible, it is sufficient to choose one or more filters using the dropdown menu and the table is automatically filtered. It is possible to remove one filter at a time by clicking on it, or to remove all the filters at the same time by clicking on the  icon, as show in the following picture.

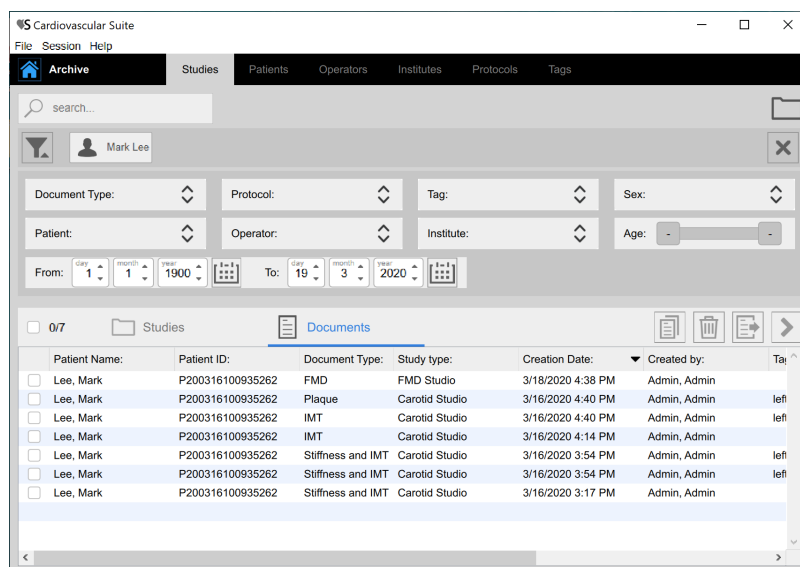


9.7.2 Management of Studies Table


Selecting the Studies tab , the Studies table is shown where you can find the list of all the studies performed and stored into the Archive.

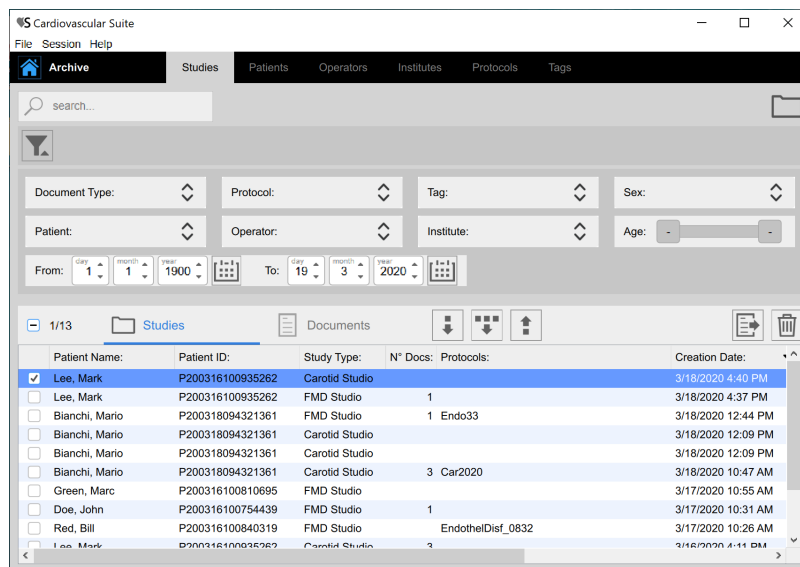


Import a study:

- Click on the Import Study  button that is placed on the top of the Studies Table.
- Select the folder that contains the study to be imported, then press Open.

Import more than one study:


- Click on the Multiple Import Study  button that is placed on the top of the Studies Table.
- Select the folder that contains the studies to be imported, then select the studied and press Open.

Export a study:

- In table (4), click on the study to be exported.
- Click on the Export Study  button that is placed on the left of the Studies Table.
- Select the destination path where you want to save your exported study, then press Save.

A report file in CVS format is created in the destination folder. It contains the details of the exported study.

Delete a study:

- In table (4), click on the study to be deleted.
- Click on the Delete Study  button that is placed above the Studies Table, on the right.

Multiple selection:

In Studies Table multi-select feature is available. You can select more than one study and perform export and delete operation on selected studies.


In table (4), select the studies through the check-box. The label over the table shows how many studies are selected from the available ones.

After you have selected studies you can export them (clicking on multiple Export  button, placed above the Studies Table) or delete them (clicking on Delete  button, placed above the Studies Table, on the right).

Advanced export:






It is possible to export documents of selected study/studies as CSV, TSV or PDF file.

- In table (4), select the study/studies to be exported

- Click on the Export Documents  button that is placed on the top of Studies Table. A drop-down menu appears:
 - *Export Document Results*: it exports a TSV/CSV file containing information about the study, the document, and the computed results. You can also export a PDF report of the document.
 - *Export Document Data*: it exports a TSV/CSV file containing the results of the study and the instantaneous data.
- Select the destination path where you want to save your exported documents, then press Save.


9.7.2.1 Study view

It is possible to open the study view by double clicking on it from the Studies Table **(4)**. A new window containing the study and its files is opened, as shown in the following picture. Some buttons are also available to operate the study:






- Click the next  or to the previous  study button to navigate among the studies.
- Click the Generate study report  button to create a PDF report of the study (available for Carotid Stdio only, see [Study report](#)).
- Click the Export the Study  button to export the current study.
- Click the Delete the Study  button to delete the current study.

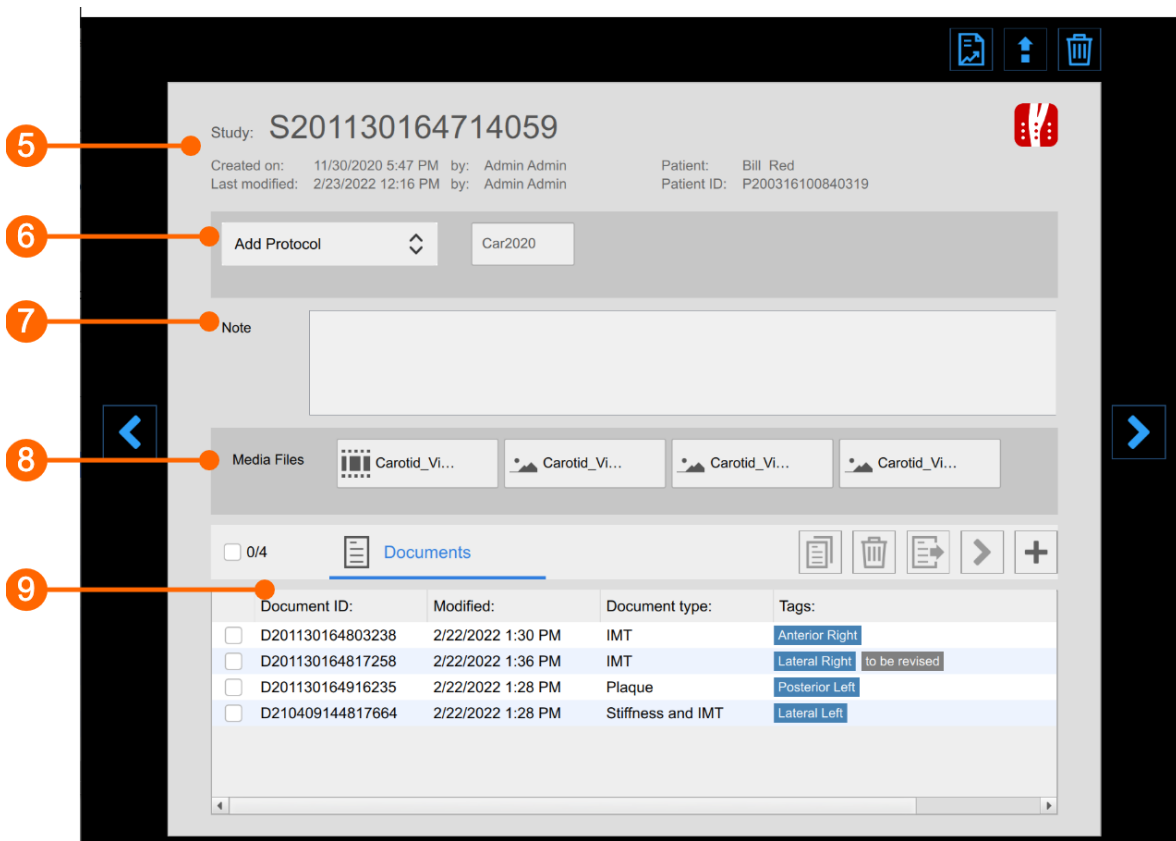The study view contains:


- a panel with information regarding the study and the patient **(5)**.
- a panel for adding and removing protocols to the study **(6)**.
- a note text field **(7)** where it is possible to add comments to the study.
- a media file container **(8)** which collects all the media files of the study (clicking on the media file icon new window for showing the file is opened).
- a table containing all the study documents and the buttons **(9)** for managing them.




It is possible to click on a document of the table to see some information about the document itself.


From the documents table (9) it is also possible to create a new document related to that study, by clicking on the  button. You can select one or more document and duplicate one of them using the duplicate  button. For selected documents, it is also possible to export  and delete  them. In addition, by clicking on the  icon it is possible to view the review of that document.

9.7.3 Management of Documents Table


Selecting the Documents tab , the Documents table is shown.

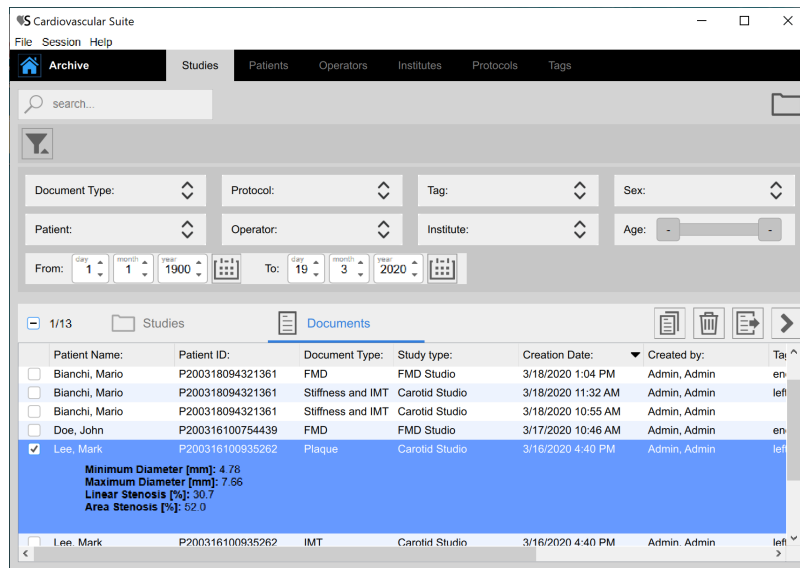

Open a document:

- Click on the document to be open.
- Click on the Go  button in document preview and the document will open in the application that created it or,
- Double click on the document to be open.
- The document will open in the application that created it.

Duplicate a document:


- In the Documents table, click on the document to be duplicated.
- Click on the Duplicate Document  button placed above the table.

Delete a document:

- In the Documents table, click on the document to be deleted.
- Click on the Delete Document  button placed above the table.

Export a document:



It is possible to export one or more documents as CSV, TSV or PDF file.

- In the Documents table, select the document to be exported.
- Click on the Export Document  button, placed above the Documents table. A drop-down menu appears:
 - Export Document Results*: it exports a TSV/CSV file containing information about the study, the document, and the computed results. You can also export a PDF report of the document.
 - Export Document Data*: it exports a TSV/CSV file containing the results of the study and the instantaneous data.
 - Export Aggregated Results* (available only if more than a document is selected): it is also possible to export aggregated results of different documents in a single CSV or TSV file (please note that selected studies should all be of the same type).
- Select the destination path where you want to save your exported documents, then press Save.

Multiple selection:


In Documents Table multi-select feature is available. You can select more than one document and perform export and delete operation on selected documents.

In table, select the documents through the check-box. The label over the table shows how many documents are selected from the available ones.

After you have selected documents you can export them (clicking on Export  button) or delete them (clicking on Delete  button).

9.8 Patients management

Allows you to manage patients.

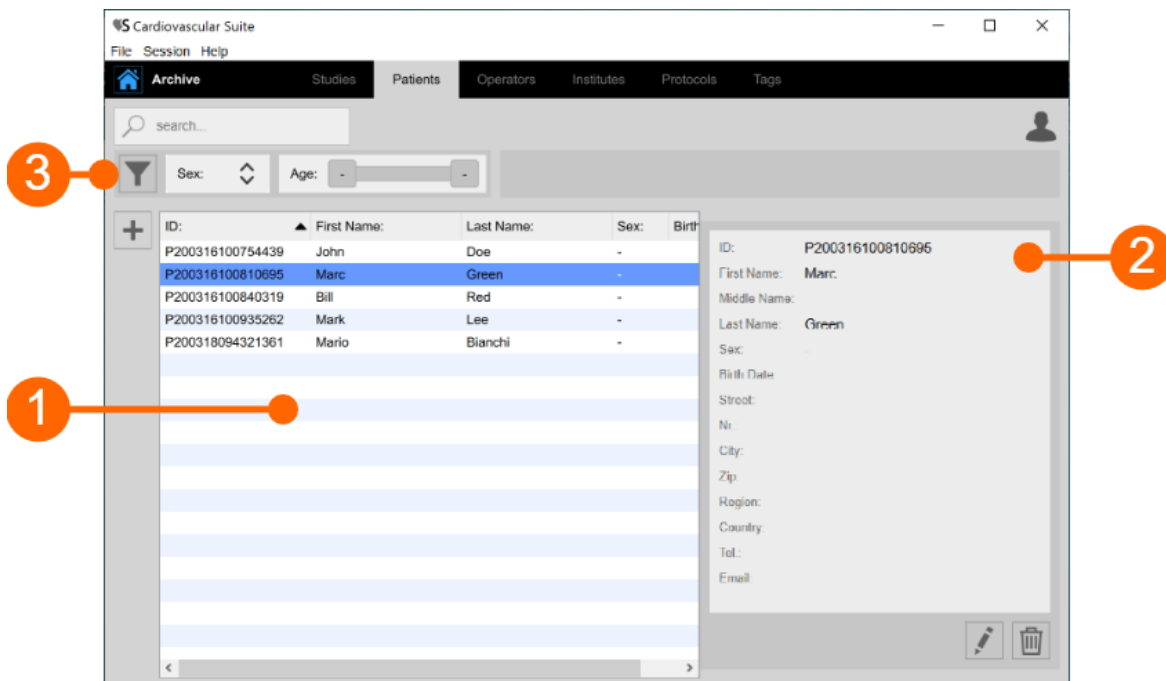

The patient list is given in table **(1)**. Once you select one of patients, detailed information are shown in the frame **(2)**.

In the frame **(3)** you can perform textual research and add and remove filters. The following filter can be used:

- Sex
- Age

In addition, with a double click on a patient, the list of the study related to that patient is shown in the [Studies management](#) window:



Cardiovascular Suite

File Session Help

Archive Studies Patients Operators Institutes Protocols Tags

search...

Mark Lee

Document Type: Protocol: Tag: Sex:

Patient: Operator: Institute: Age:



From: 1 1 1900 To: 19 3 2020

0/7 Studies Documents




Patient Name:	Patient ID:	Document Type:	Study type:	Creation Date:	Created by:	Tag:
<input type="checkbox"/> Lee, Mark	P200316100935262	FMD	FMD Studio	3/18/2020 4:38 PM	Admin, Admin	
<input type="checkbox"/> Lee, Mark	P200316100935262	Plaque	Carotid Studio	3/16/2020 4:40 PM	Admin, Admin	left
<input type="checkbox"/> Lee, Mark	P200316100935262	IMT	Carotid Studio	3/16/2020 4:40 PM	Admin, Admin	left
<input type="checkbox"/> Lee, Mark	P200316100935262	IMT	Carotid Studio	3/16/2020 4:14 PM	Admin, Admin	
<input type="checkbox"/> Lee, Mark	P200316100935262	Stiffness and IMT	Carotid Studio	3/16/2020 3:54 PM	Admin, Admin	left
<input type="checkbox"/> Lee, Mark	P200316100935262	Stiffness and IMT	Carotid Studio	3/16/2020 3:54 PM	Admin, Admin	left
<input type="checkbox"/> Lee, Mark	P200316100935262	Stiffness and IMT	Carotid Studio	3/16/2020 3:17 PM	Admin, Admin	




Add a new patient:


- Click on the Add New Patient  button.
- In the new patient frame (4), enter the patient data. The only mandatory field is the patient ID and the software automatically creates a new one.
- Click on the Save  button to save the patient data.

Modify a patient:

- Select the patient to be modified.
- Click on the Edit  button.
- Modify the patient data in the frame (5).
- Click on the Save  button to save the data.
- You can use the Restore  button to restore data.


Delete a patient:

- Select the patient to be deleted.
- Click on the Delete  button.
- Confirm deletion with the OK button.

 You cannot delete a patient that is associated with existing studies.


9.9 Operators management

Allows you to manage operators.

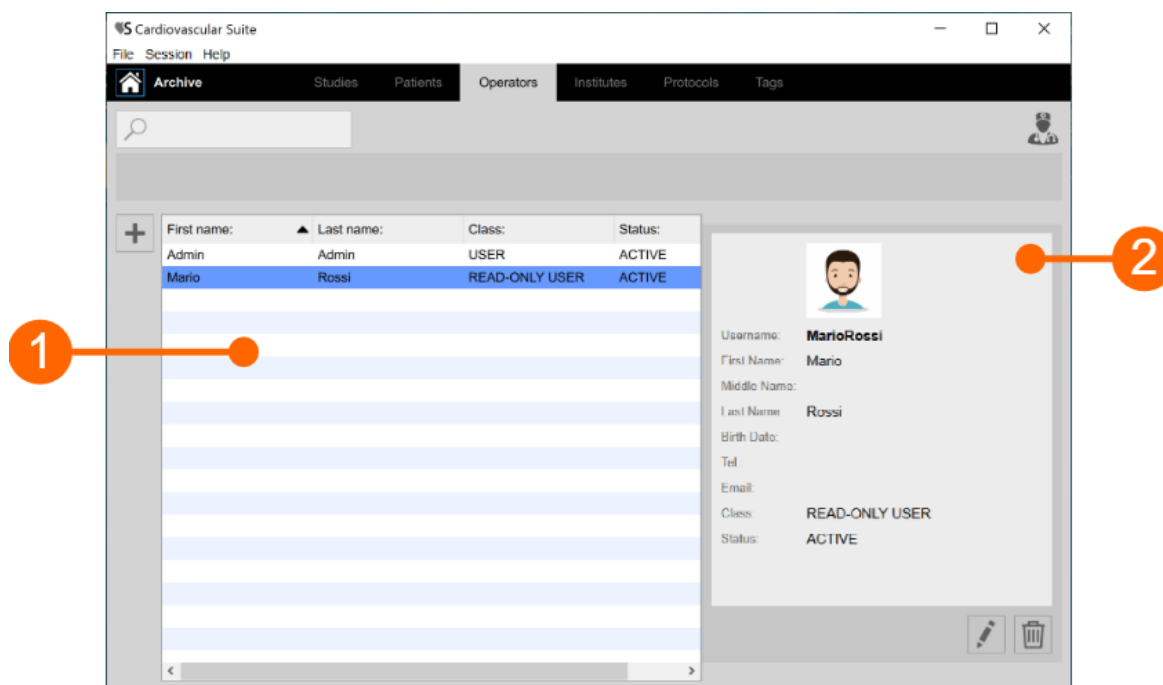



The operators list is given in the table above **(1)**. Once you select one of the operators, detailed information are shown in the frame **(2)**.

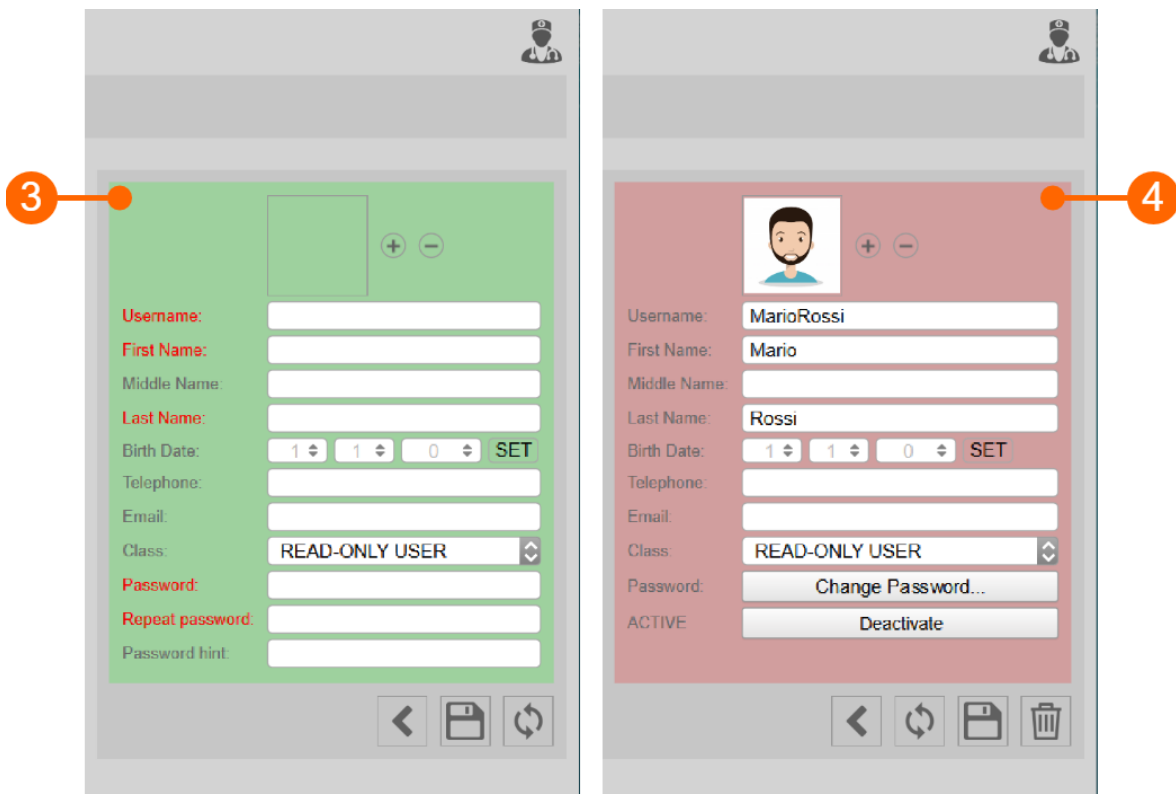


You can double click on the operator in table **(1)** to show the studies performed by this operator in the [Studies management](#) window.




Add a new operator:


- Click on the Add New Operator  button.
- In the new operator frame (3), enter the operator data. Labels of mandatory fields (First Name, Last Name) are red.
- Click on the Save  button to save the operator data.

Modify an operator:

- Select the operator to be modified.
- Click on the Edit  button.
- Modify the operator data in the frame (4).
- Click on the Save  button to save the data.
- You can use the Restore  button to restore data.


Delete an operator:

- Select the operator to be deleted.
- Click on the Delete  button.
- Confirm deletion with the OK button.

 You cannot delete an operator that is associated with existing studies.


9.10 Institutes management

Allows you to manage institutes.

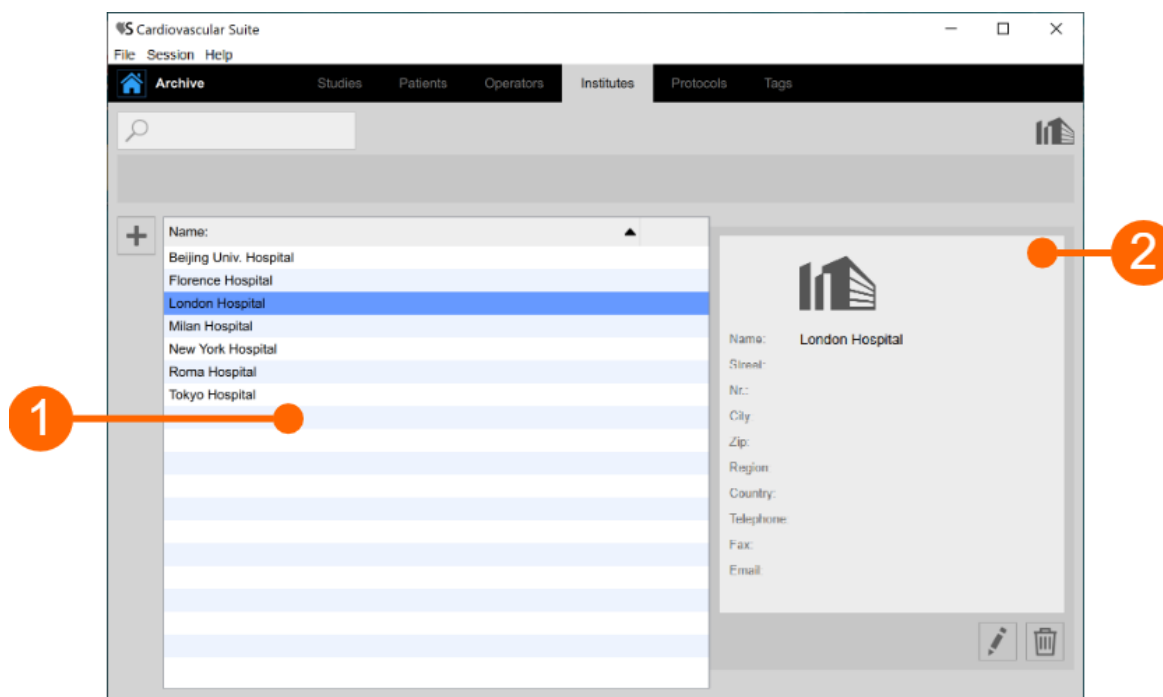



The institutes list is given in table **(1)**. Once you select one of the institutes, detailed information are shown in the frame **(2)**.

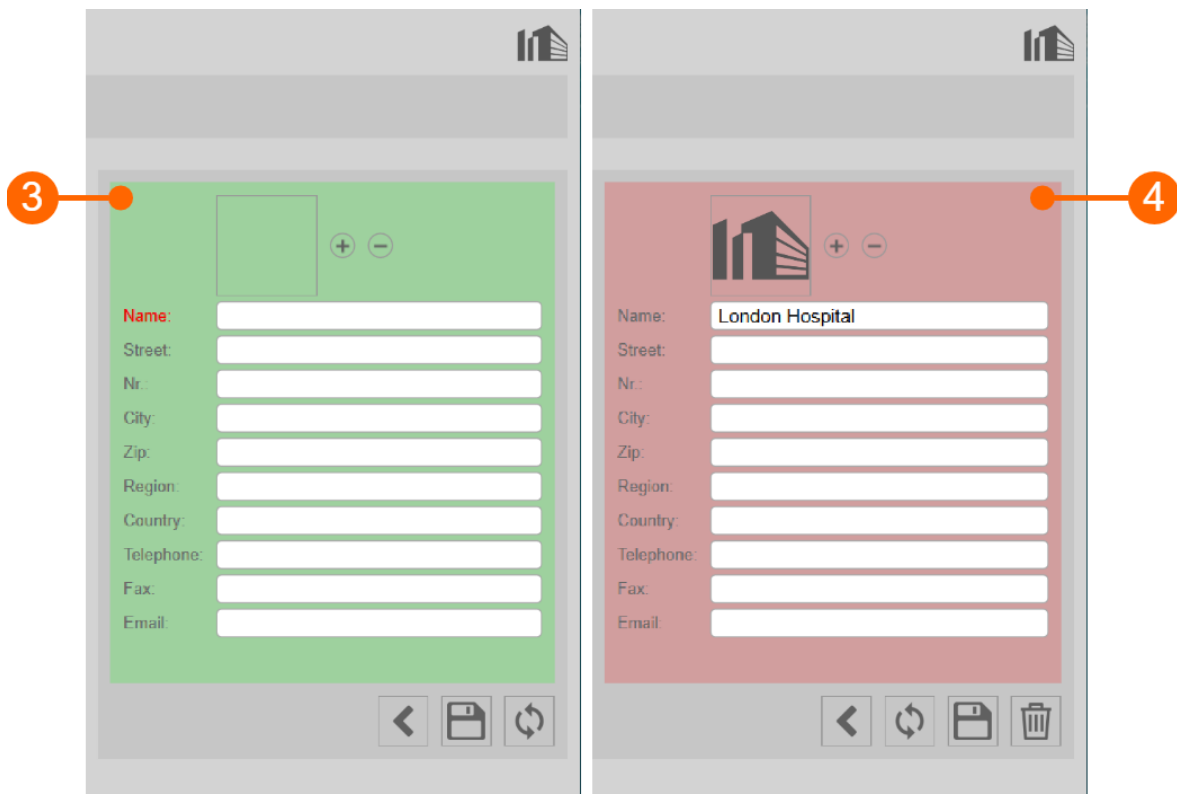


You can double click on the institute in table **(1)** to show the studies performed within this institute in the [Studies management](#) window.




Add a new institute:


- Click on the  button for adding a new institute.
- In the new institute frame **(3)**, enter the institute data. The mandatory field (Name) is in red.
- Click on the Save  button to save the institute data.

Modify an institute:

- Select the institute to be modified.
- Click on the Edit  button.
- Modify the institute data in the frame **(4)**.
- Click on the Save  button to save the data.
- You can use the Restore  button to restore data.


Delete an institute:

- Select the institute to be deleted.
- Click on the Delete  button.
- Confirm deletion with the OK button.

 You cannot delete an institute that is associated with existing studies.


9.11 Protocols managements

Allows you to manage protocols.

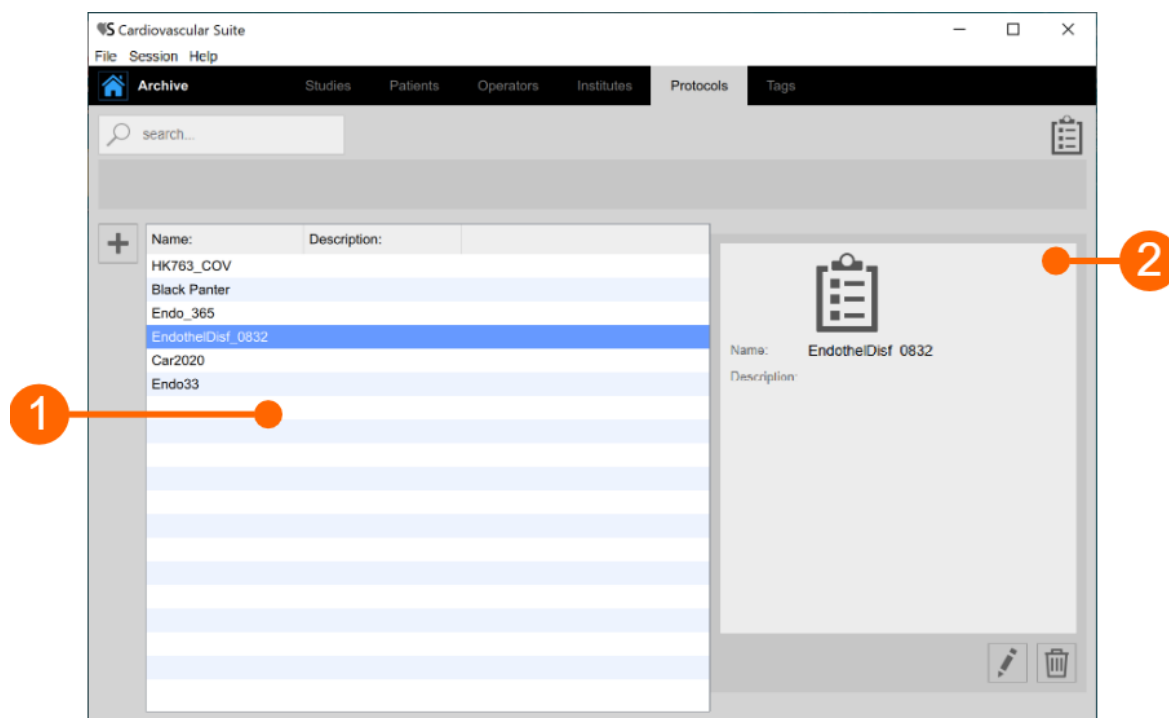



The protocols list is given in table (1). Once you select one of the protocols, detailed information are shown in the frame (2). At the top of the screen there is a search field to perform a textual research for protocols in the list.

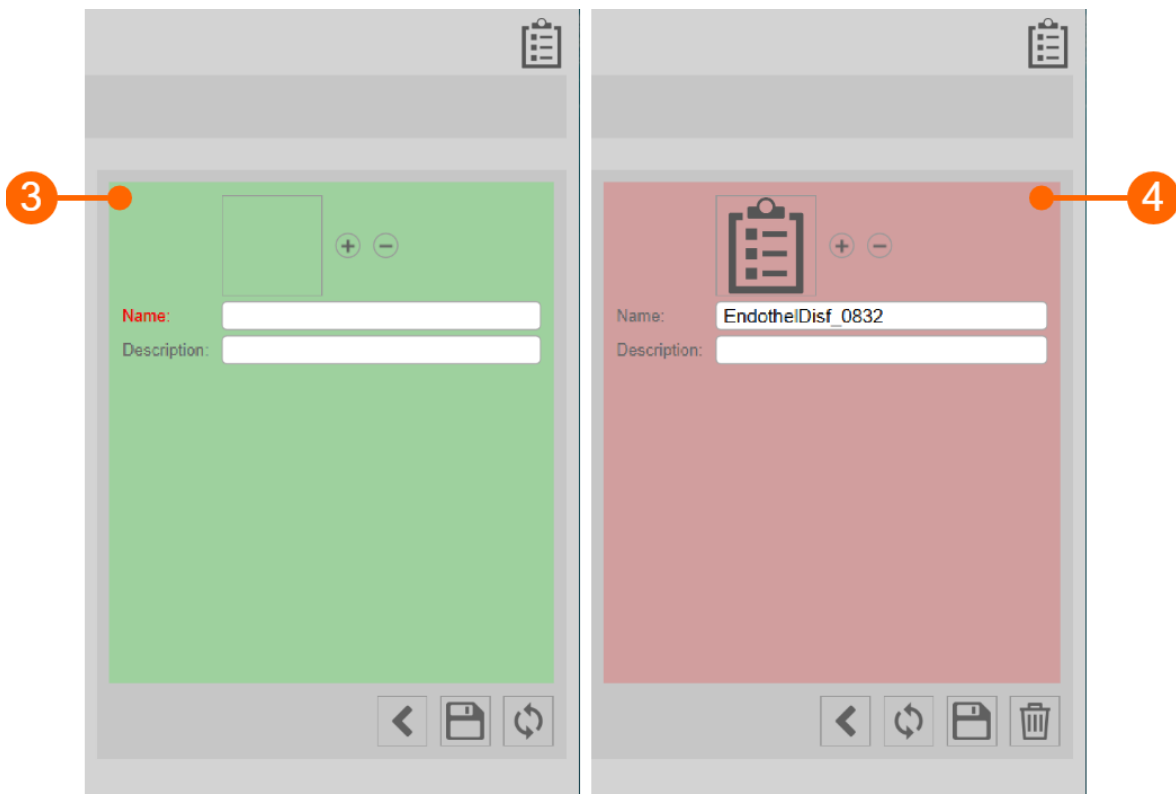


You can double click on the protocol in table (1) to show the studies performed within this protocol in the [Studies management](#) window.




Add a new protocol:


- Click on the  button for adding a new protocol.
- In the new protocol frame **(3)**, enter the protocol data. The mandatory field (Name) is in red.
- Click on the Save  button to save the protocol data.

Modify a protocol:

- Select the protocol to be modified.
- Click on the Edit  button.
- Modify the protocol data in the frame **(4)**.
- Click on the Save  button to save the data.
- You can use the Restore  button to restore data.


Delete a protocol:

- Select the protocol to be deleted.
- Click on the Delete  button.
- Confirm deletion with the OK button.

 You cannot delete a protocol that is associated with existing studies.


9.12 Tags management

The Archive Tags section allows you to manage the custom tags.

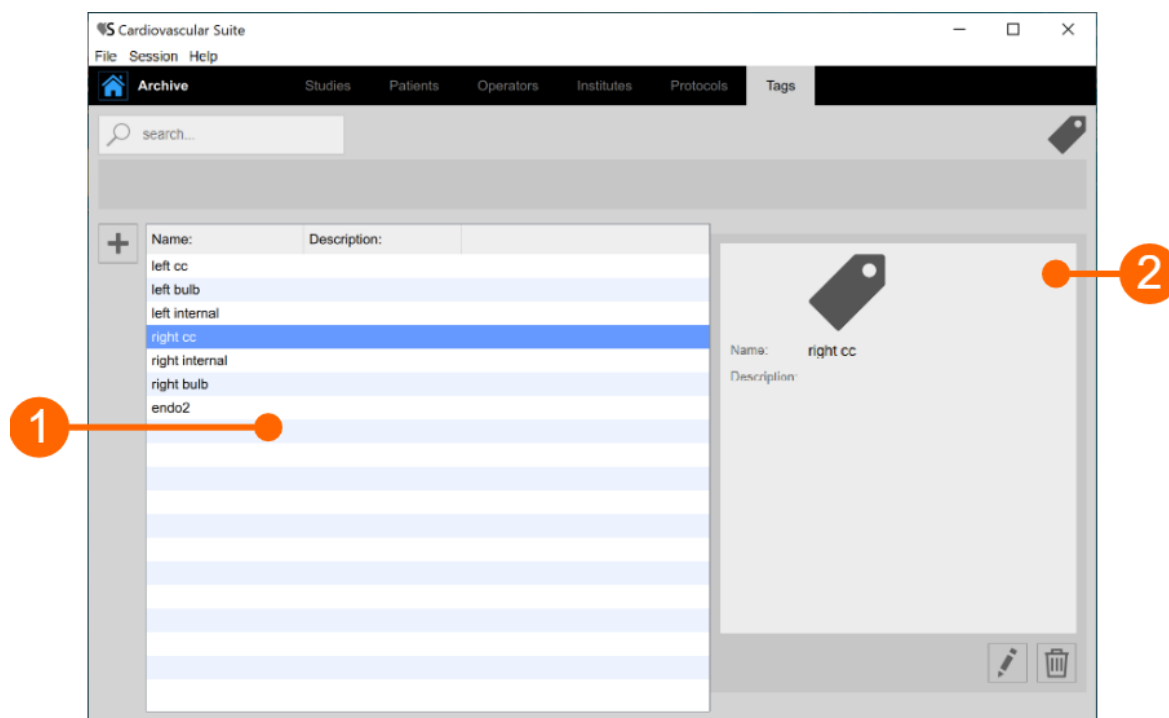



The tags list is given in table **(1)**. Once you select one of the tags, detailed information are shown in the frame **(2)**. At the top of the screen there is a search field to perform a textual research for tags in the list.

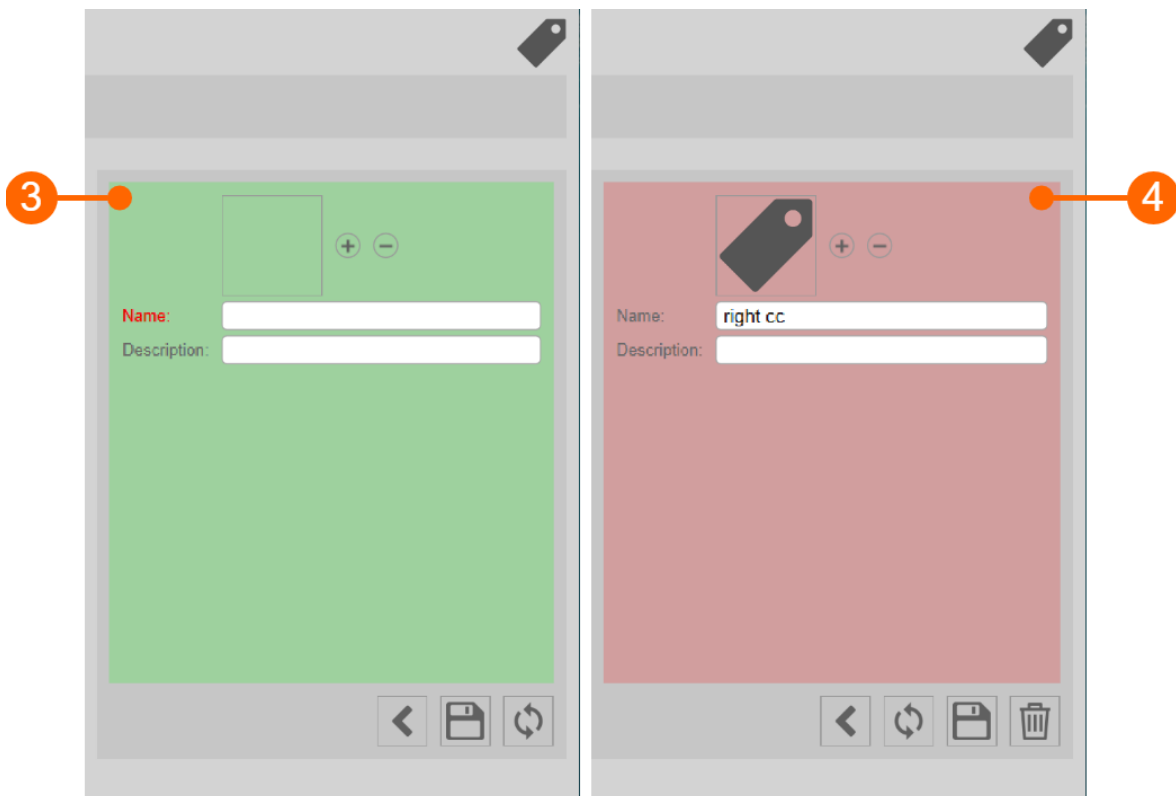


You can double click on the tag in table **(1)** to show the documents associated to this tag in the [Studies management](#) window.




Add a new tag:


- Click on the  button for adding a new tag.
- In the new tag frame **(3)**, enter the tag data. The mandatory field (Name) is in red.
- Click on the Save  button to save the tag data.

Modify a tag:

- Select the tag to be modified.
- Click on the Edit  button.
- Modify the tag data in the frame **(4)**.
- Click on the Save  button to save the data.
- You can use the Restore  button to restore data.

Delete a tag:

- Select the tag to be deleted.
- Click on the Delete  button.
- Confirm deletion with the OK button.

 You cannot delete a tag that is associated with existing documents.


10 Carotid Studio

Carotid Studio is a software for the measurement of the Intima Media Thickness (IMT), the carotid diameter, and the stiffness parameters by processing sequences of ultrasound images. On single images, the software also provides a tool for the measurement of geometric and statistic parameters on plaques that are recognized manually by the operator.

10.1 Create a new study


When you start Carotid Studio, a procedure guides you in the creation of a new study. The steps are:

10.1.1 Select the study modality

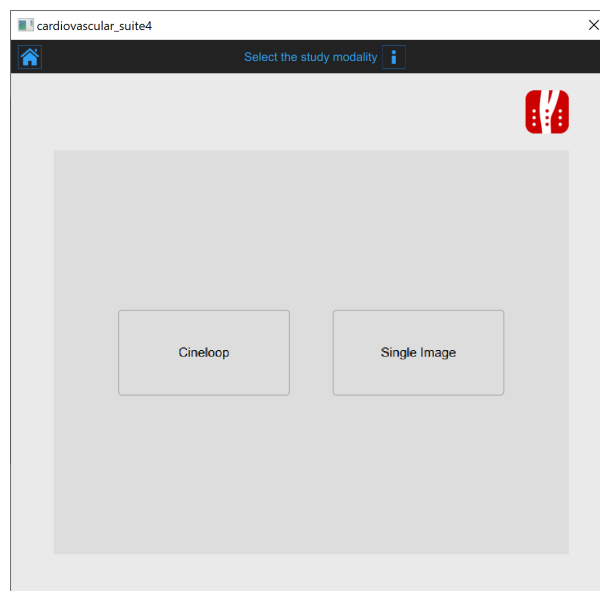

In this tab, you can select the study modality. Carotid Studio allows to analyze through "Cineloop" modality (loading a video clip) and "Single Image" modality (processing a single frame coming from a video or loaded as image).


10.1.2 Select the source

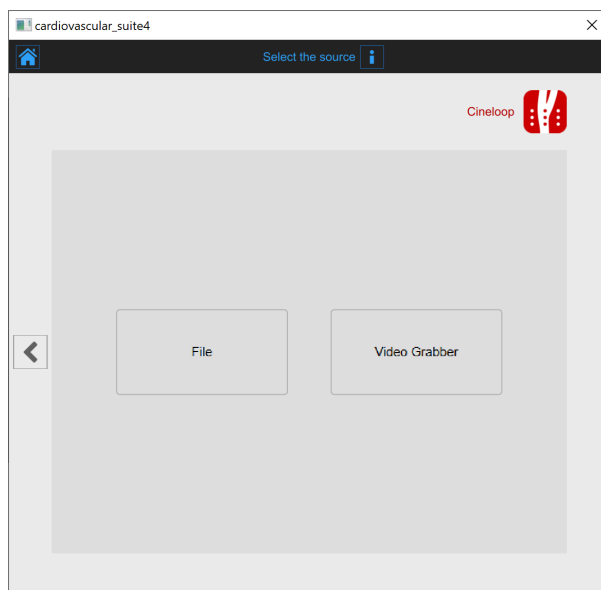




In this tab, you can select the study video source. With the "Cineloop" modality, Carotid Studio processes video sources (Video File or a DICOM File) while with "Single Image" it also processes images. Both the modalities allow to work in real-time by processing images directly coming from the ultrasound equipment thanks to a video converter.


10.1.3 Select the patient

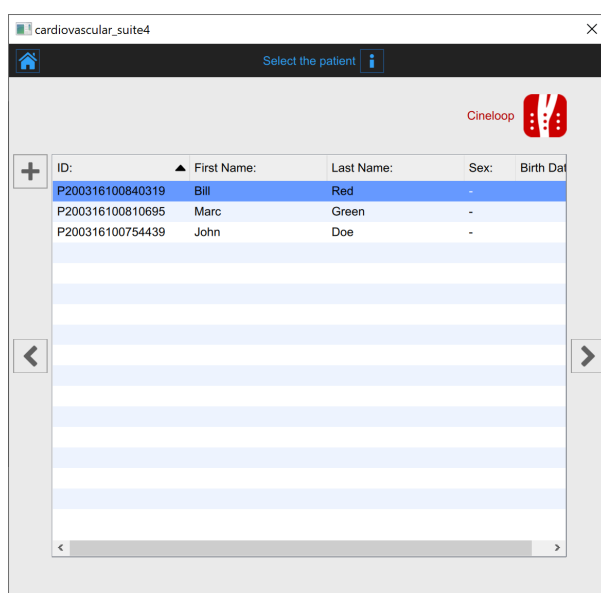i For DICOM files, the patient data are obtained by the file metadata and this window is skipped (see [Settings](#)). You can anyhow edit the patient data from the Review window.




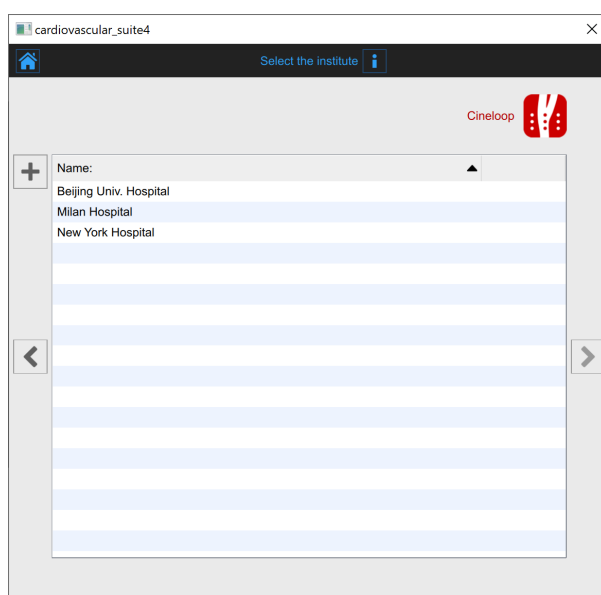
In this tab, you can select the patient among the ones already present in the [Archive](#). Select the patient and click on the Next  button (you can simply double-click on the patient to proceed). If you want to create a new patient, click of the Add New Patient  button.


In the Add new patient frame, enter the patient data. The only mandatory field is the patient ID (a random value is automatically proposed). Click on the Save button  to save the patient data.

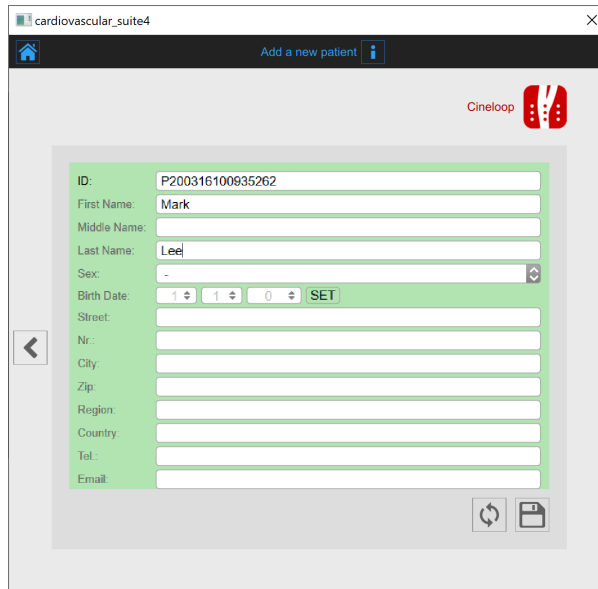


10.1.4 Select the institute


-  If it is the first time you create a study, after selecting the patient you will also need to select the institute. If you have already created at least one study, the software remembers the institute used for the previous study and after selecting the patient shows you automatically the final review (where you can still make changes before starting the new study).




In this tab, you can select the institute among the ones already present in the [Archive](#). Select the institute and click on the Next  button (you can simply double-click on the institute to proceed).



If you want to create a new institute, click of the Add New Institute  button.

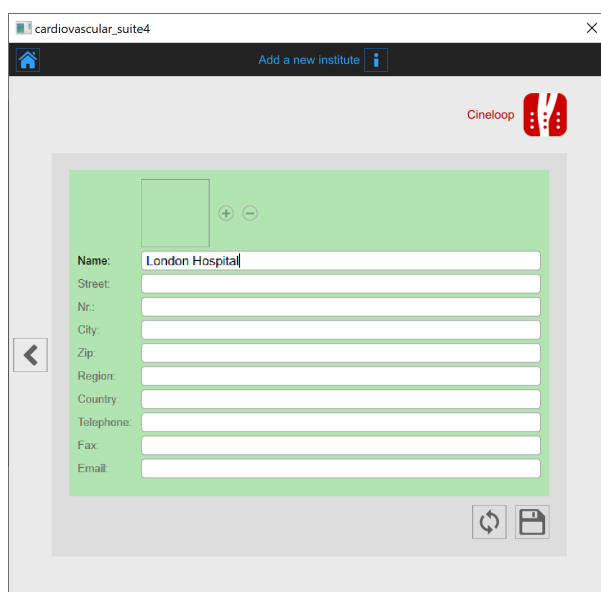
In the Add new institute frame, enter the institute data. The mandatory field (Name) is in red until you have filled in the Name blank. Click on the Save  button to save the institute data.




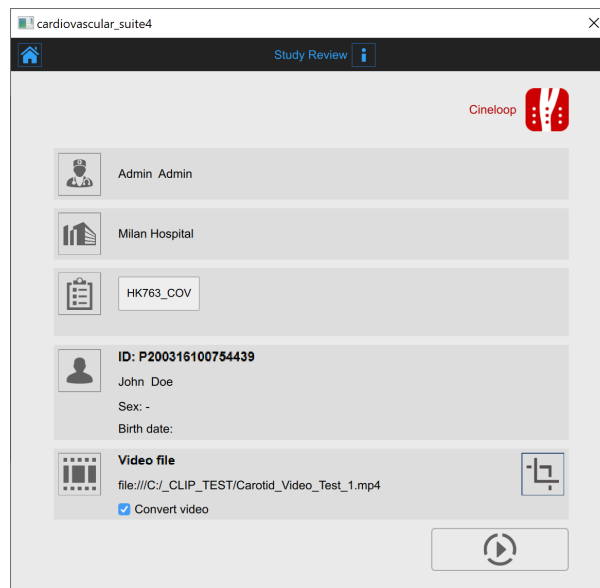

10.1.5 Review





In this tab you can review your selection (you can also change Patient  and Institute  by clicking on their buttons). It is possible also to change the selected source for this study by clicking on the icon that represents the source.

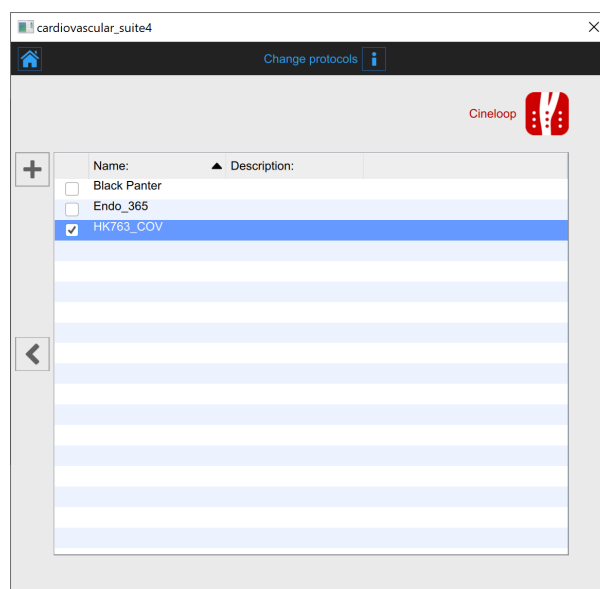
Here, the user has the possibility to associate the study to one or more existing protocols, by clicking on the protocols icon .




In the Protocols tab, you can associate the study to one or more than one protocols already present in the Archive. Put a tick on the protocol you want to associate the study with. If you want to create a new protocol, click of the Add New protocol  button. In the Add new protocol frame, enter the protocol data. The mandatory field (Name) is in red until you have filled in the Name blank. Click on the Save  button to save the protocol data.

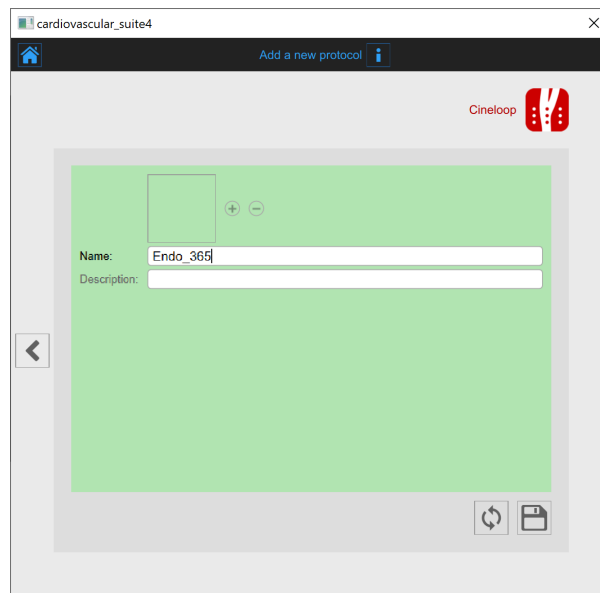



Click on the Previous  button to go back to the review window.


-  If in the [Settings manager](#) the option "Remember last used protocols" is checked, the study will be associated by default with the last used protocols.


In addition, if you have chosen a video file as source, in the review window, it is possible to convert the video file to be optimized for the analysis with Carotid Studio. This operation may take few minutes.

-  The default value of the "Convert video" checkbox is set by the "Convert video by default" option in the [Settings manager](#).


You can also crop the images by clicking the Crop  button in the source panel. In this case, a new window opens; it is possible to select a region to be used for the analysis. Click on the Confirm  button after you have drawn the region.



Click on the Start the Study  button to proceed. A progress bar, as shown in the following picture, will show you the progression of the study creation.

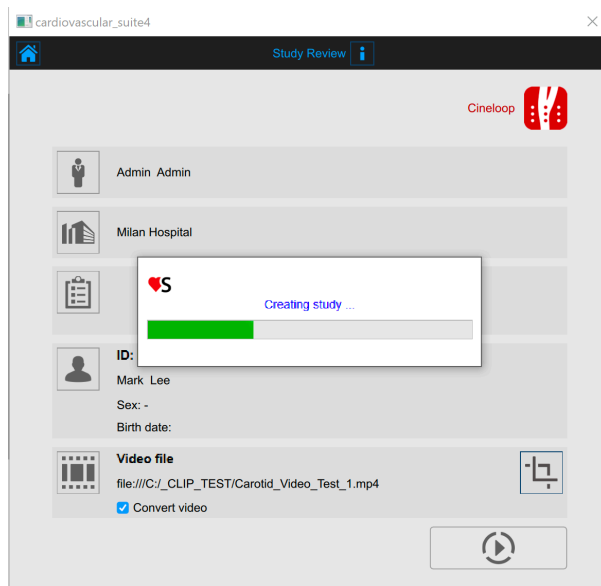

10.2 Cineloop study analysis

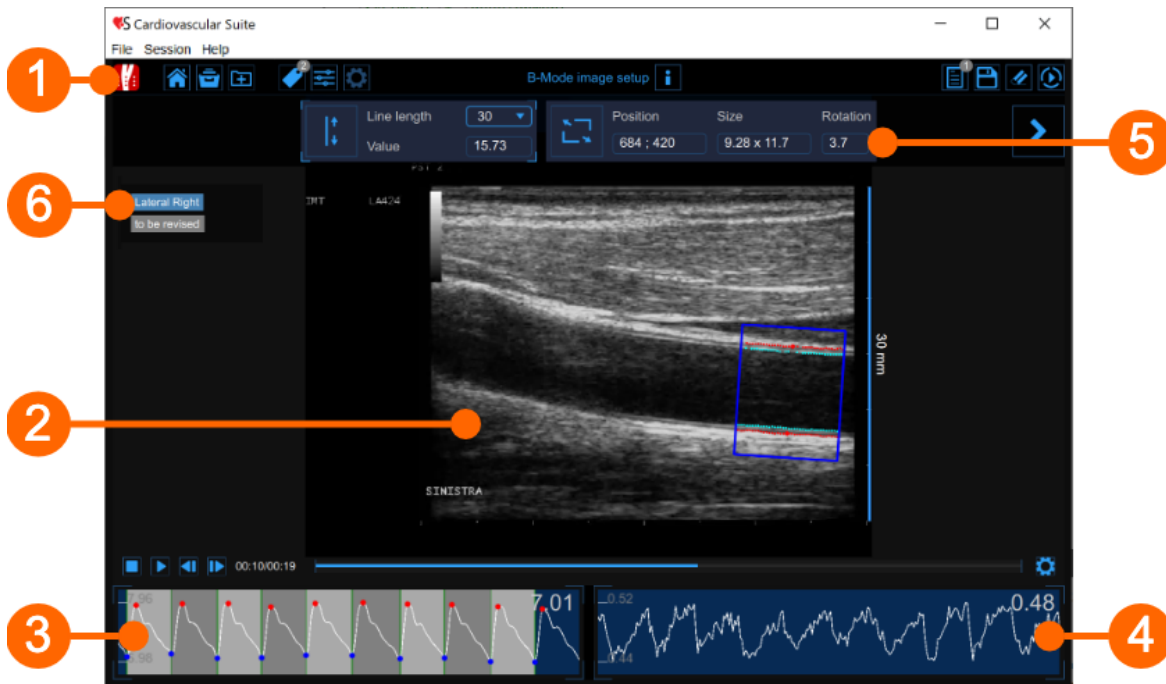


The analysis window contains the following components:


1. Top bar
2. Video window
3. Diameter chart
4. IMT chart
5. Setup panel
6. Tags


10.2.1 Top bar

The top bar contains some essential information for the navigation. Several icons are displayed.



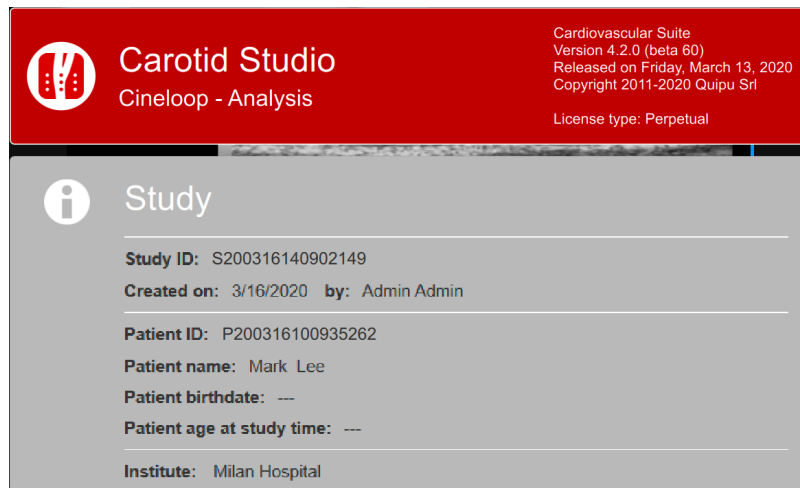

The Carotid Studio  button shows information about the study and about Cardiovascular Suite. Regarding the study, the number identification (ID) is displayed together with information about patient and the institute. Information about the software such as version and type of license are shown in the upper part of the windows, as the following figure:





The Home button  closes the Carotid Studio application and returns to the home screen of Cardiovascular Suite.


The Archive button  closes the Carotid Studio application and returns to the archive of Cardiovascular Suite.



The New video button  allow to open a new video for the analysis.



The Tags Management button  opens the tag management panel as described in [Tags](#).


The Preset Management  button opens the preset management panel as described in [Presets](#).

The Setup Panel  button is used to show the setup panel when it is hidden.


The Info  button shows information about active controls (calibration lines, ROI, etc.).

The Start Exam  button starts the examination. While the analysis is collecting data, a red led  advises that the recording is in progress.

The Save  button saves a document of the study. With the Cancel  button it is possible to cancel the analysis and delete data in the Diameter and IMT charts.

The Review Documents  button allows to suspend the analysis and to review the documents saved in the current analysis session. The button is only activated if you saved at least one document.

10.2.2 Video window

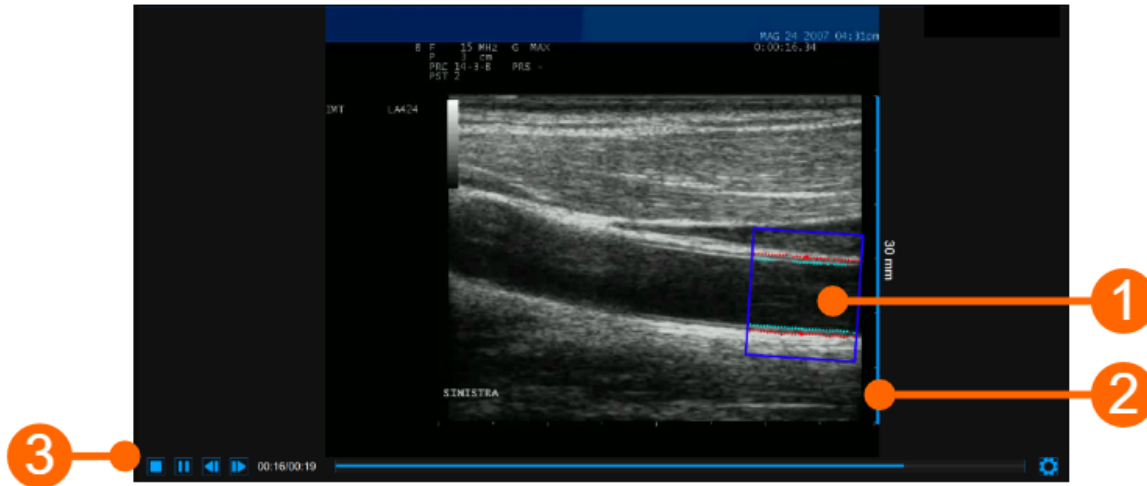


The video window shows the video signal from your ultrasound system. A ROI **(1)** can be traced in the video windows, where both the IMT and the diameter are computed.

The window also contains the calibration line **(2)** for the B-mode image once it has been calibrated. The video controls bar **(3)** is located at the bottom of the window. For more information on the video controls, see [Video and image player](#).

10.2.2.1 ROI


The Region of Interest (ROI) is the portion of the image where both the diameter and the IMT are calculated. The points of the Lumen-Intima interface and the Media-Adventitia interface are displayed within the ROI in cyan and red color respectively. The ROI can be moved, resized, and/or rotated. Each time you change the position, size and/or inclination of the ROI, the analysis is re-initialized.

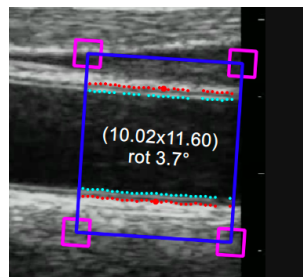

Draw a new ROI:


You can manually draw the diameter ROI with the desired size and position. If the image is already calibrated, you can also more quickly draw a diameter ROI with the default sizes set in [Carotid Studio settings](#) (a star in the Set ROI button will indicate that the default ROI can be drawn). The default ROI is also automatically rotated so to be parallel to the carotid artery.

default ROI drawing

- Click on the Set ROI  button in the [Setup panel](#) (the button remains active)
- Click in the video window in the center of the carotid artery.


- A ROI of the default ROI sizes will be automatically initialized.

manual drawing

- Click on the Set ROI  button in the [Setup panel](#) (the button remains active).
- Click inside the video window and drag until the ROI is complete (the size of the ROI is shown in the [Setup panel](#) and graphically within the ROI).
- When you release the mouse, the analysis is initialized.

Rotate the ROI:


- Click on the upper side of the ROI and use the special cursor that indicates a rotation.
- Hold inside the ROI, drag the rectangle by rotating it to the desired angle.


 As an alternative, you can modify the position of the ROI by typing the value in the [Setup panel](#).



Resize the ROI:


- Click on one of the sides or one of the corners of the ROI.
- Drag to change the size of the the ROI.


 An alternative, you can modify the size of the ROI by typing the value in the [Setup panel](#).



Move the ROI:

- Click and hold inside the ROI.
- Drag the ROI to the location of interest.


 As an alternative, you can modify the position of the ROI by typing the value in the [Setup panel](#).



Re-initialize the ROI:


- Double click inside the Diameter ROI to re-initialize the position and the rotation of the ROI

10.2.3 Diameter chart

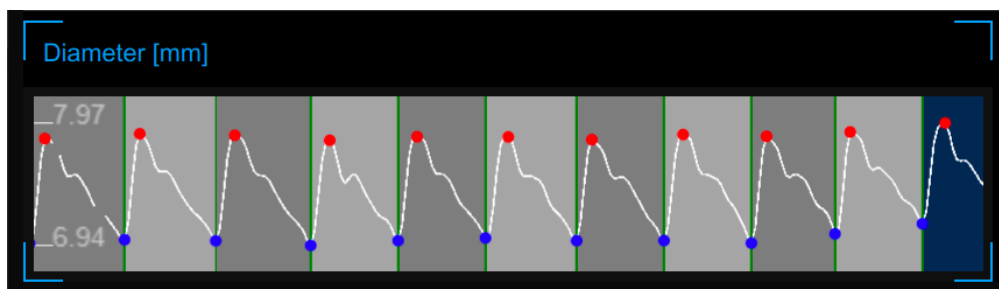

The chart shows the trend of the diameter during the examination. During the analysis, Carotid Studio recognizes the heart cycles that are shown in dark and light gray alternatively. The red points in the chart are the systolic diameters and the blue points are the diastolic diameters.

10.2.4 IMT chart

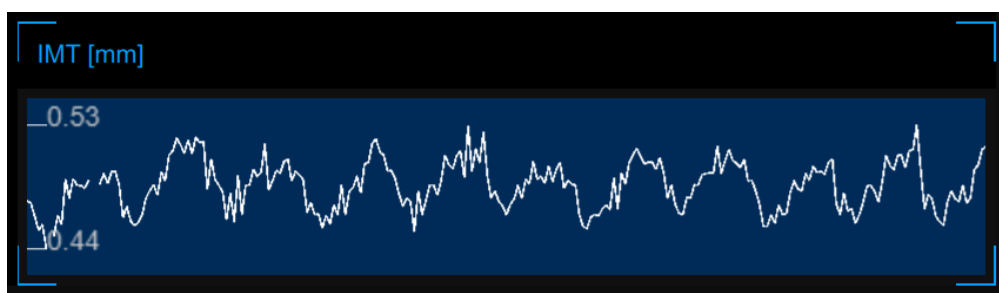

The chart shows the trend of the IMT during the examination.


10.2.5 Setup panel



The setup panel must be used to set the recording data length, to [Calibrate the B-mode image](#), to set the ROI, the *sensitivity* of the algorithm and the systolic and diastolic blood pressures.

10.2.5.1 B-mode image setup


Calibration

The Set Calibration  button is used to [Calibrate the B-mode image](#).

The drop-down menu **(1)** shows the length of the line used for the calibration.


The numeric display **(2)** shows the calibration value.

- (i)** If you click in the value field, you are allowed to manually enter the calibration value in the editable field (if you already know the value). The click the Save button to enter the values.



A screenshot of a dark-themed UI element. It features a label 'VALUE' followed by a text input field containing the number '15.77'. To the right of the input field are two small square buttons: one with a blue 'X' and one with a blue checkmark.


ROI

The Set ROI  button is used to set the ROI.

The numeric display **(3)** shows the center position, in pixels, of the ROI.

The numeric display **(4)** shows the size (width x height), in pixels, of the ROI.

- (i)** If you click in the value field, you are allowed to manually enter the ROI position and size values in the editable fields (if you already know the values). The click the Save button to enter the values.

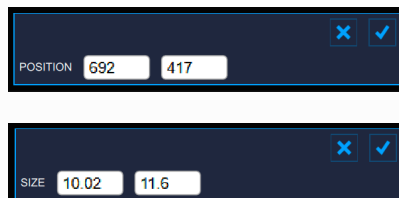

Two screenshots of dark-themed UI elements. The top one shows a label 'POSITION' followed by two text input fields containing the numbers '692' and '417'. The bottom one shows a label 'SIZE' followed by two text input fields containing the numbers '10.02' and '11.6'. Both screenshots show a blue 'X' button and a blue checkmark button to the right of the input fields.

The numeric displays **(8)** show the degree of rotation of the ROI.

- (i)** If you click in the value field, you are allowed to manually enter the degree value of rotation.



A screenshot of a dark-themed UI element. It features a label 'ROTATION' followed by a text input field containing the number '3'. To the right of the input field are two small square buttons: one with a blue 'X' and one with a blue checkmark.

Sensitivity


The slider **(5)** sets the sensitivity of the algorithm. Adjust this value in order to have a better detection of the intima-media border and the media-adventitia border.

10.2.5.2 Recording Data Length

The drop-down menu **(6)** shows the time length of the diameter and IMT data recording.

10.2.5.3 Blood Pressure



The numeric displays **(7)** show the values of systolic and diastolic blood pressure. If you click in the value field, you are allowed to manually enter the values of systolic and diastolic blood pressure. The click the Save button to enter the values.




If present, these values will be used to compute the stiffness parameters. For this purpose, the local carotid pressure should be used: in this case the carotid waveform is obtained by tonometer or similar device and it is generally calibrated by brachial measurement (sphygmomanometer) assuming that mean and diastolic values are constant along the arterial tree. For more information you can see:

"Reference values for local arterial stiffness. Part A: Carotid artery", Engelen L, Bossuyt J, Ferreira I et al., *J Hypertens.* 2015 Oct;33(10):1981-96

"Expert consensus document on arterial stiffness: methodological issues and clinical applications.", S. Laurent, J. Cockcroft, L. Van Bortel et al., *Eur Heart J.* 2006 Nov;27(21):2588-605


Once you have calibrated the B-Mode image and set the ROI, click on the Next  button to proceed to set the recording the data length and the blood pressure. Alternatively, you can click on the Start study  button to start the analysis.

10.2.6 Tags

The Tags Management  button opens a panel that allows to associate a tag to the document, or create a new tag. Carotid studio can use two types of tags:


1. System tags, which are already defined in Cardiovascular Suite. System tags are used to specify which segment of the Carotid artery is analysed, and are necessary to include the document data in the study report. Only one system tag can be associated to a document.
2. Custom tags, which are defined by the user and are used to better identify a document.

Custom tags can also be managed through the Tags management into the Archive.

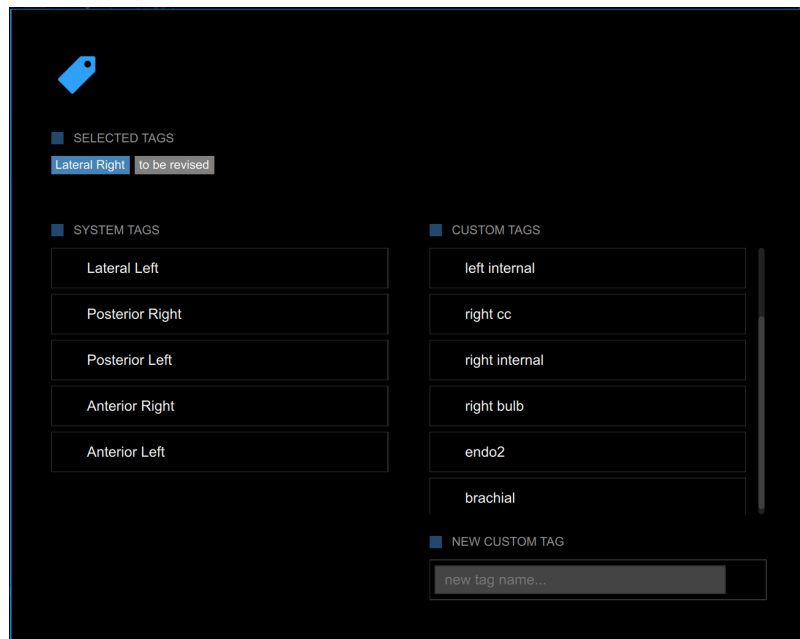


The selected tags are visible in a special area of the Analysis window. The tags area can be moved by right clicking and dragging.

10.2.7 Presets


The preset management  button opens the preset management panel that allows to manage presets. In particular, it allows to remember the settings of:

- B-mode image calibration
- B-mode image ROI (size, position, and rotation)
- recording time

A preset can be saved and reused for following studies.

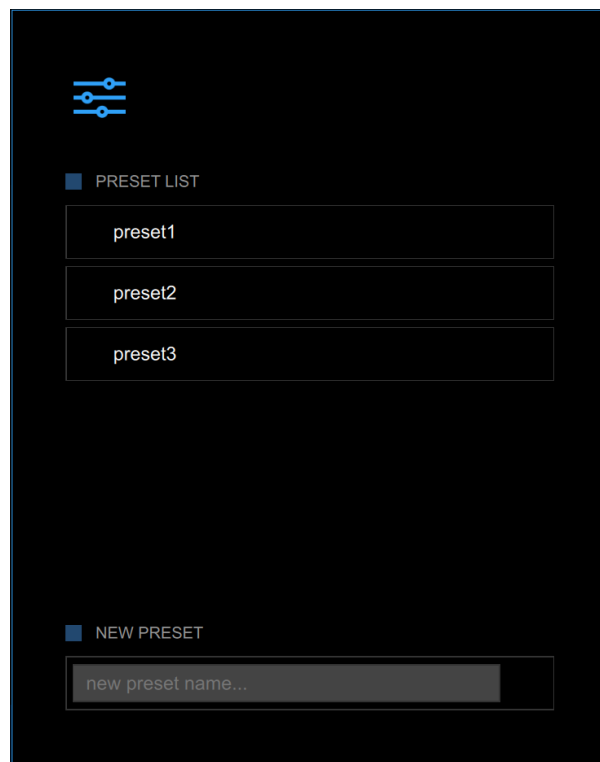

10.3 Single image study analysis

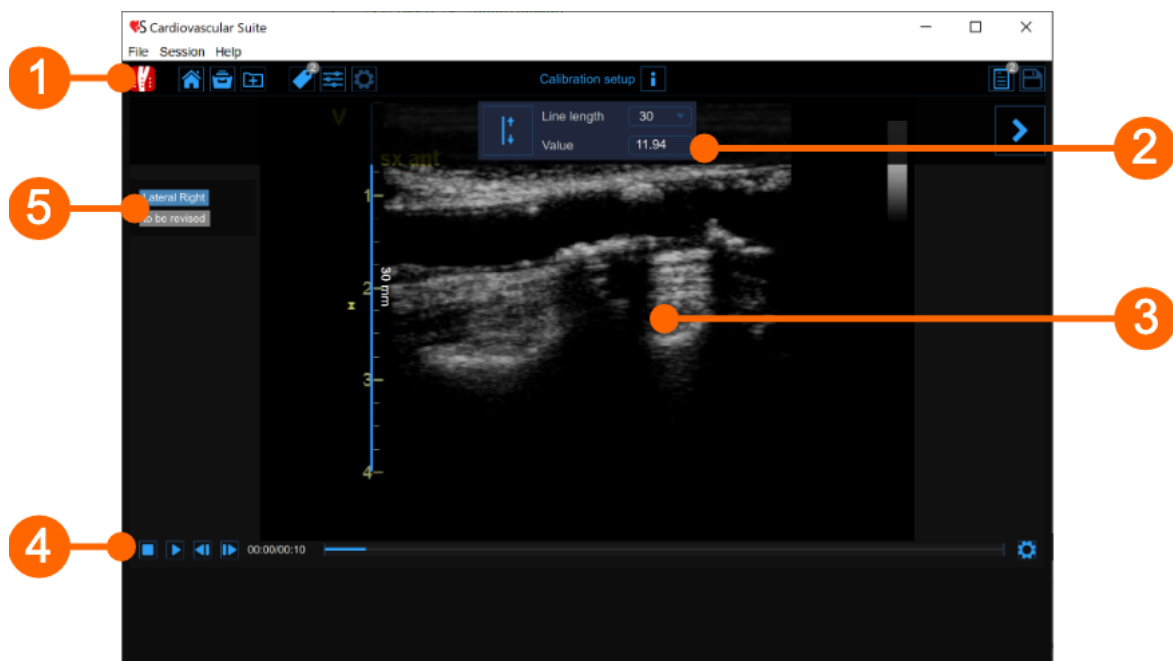


Carotid Studio single image modality analyses image files or a single image selected from a video file and allows to perform two different types of analysis:

- [IMT analysis](#)


- [Plaque analysis](#)


The single image analysis window contains the following components:


1. Top bar





The top bar contains some essential information for the navigation. Several icons are displayed.

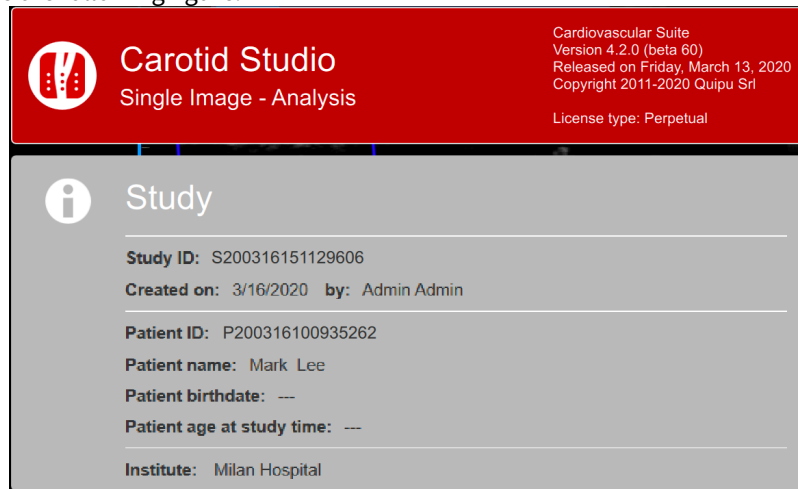
The Carotid Studio button  shows information about the study and about Cardiovascular Suite. Regarding the study, the number identification (ID) is displayed together with information about patient and the institute. Information about the software such as version and type of license are shown in the upper part of the windows, as the following figure:






The home button  closes the Carotid Studio application and returns to the home screen of Cardiovascular Suite.


The Archive button  closes the Carotid Studio application and returns to the archive of Cardiovascular Suite.


The New video/image button  allow to open a new video/image for the analysis.


The Tags Management button  opens the tag management panel as described in [Tags](#).

The preset management button  opens the preset management panel as described in [Presets](#).

The Info  button shows information about active controls (calibration lines, ROI, etc.). The  icon is used to show the setup panel when it is hidden.

The Freeze/Run  button suspends and resume the image acquisition (present in real-time analysis only).


The Save  button saves a documents of the study.

The Review Documents  button allows to suspend the analysis and to review the documents saved in the current analysis session. The button is only activated if you saved at least one document.


2. Setup panel

The setup panel must be used to [Calibrate the B-mode image](#).

Calibration

The Set Calibration  button is used to [Calibrate the B-mode image](#). The drop-down menu shows the length of the line used for the calibration. The numeric display shows the calibration value.

- i** If you click in the value field, you are allowed to manually enter the calibration value in the editable field (if you already know the value). The click the Save button to enter the values.



3. Image window

The media window shows the media file that is analyzed.


4. Image window control bar

The media window control bar is at the bottom of the media window and contains controls to manage the playback of a movie (only in case of video file) and the brightness and contrast adjustment.

5. Tags Area

The selected tags are visible in this area. The tags area can be moved by right clicking and dragging.

10.3.1 IMT analysis

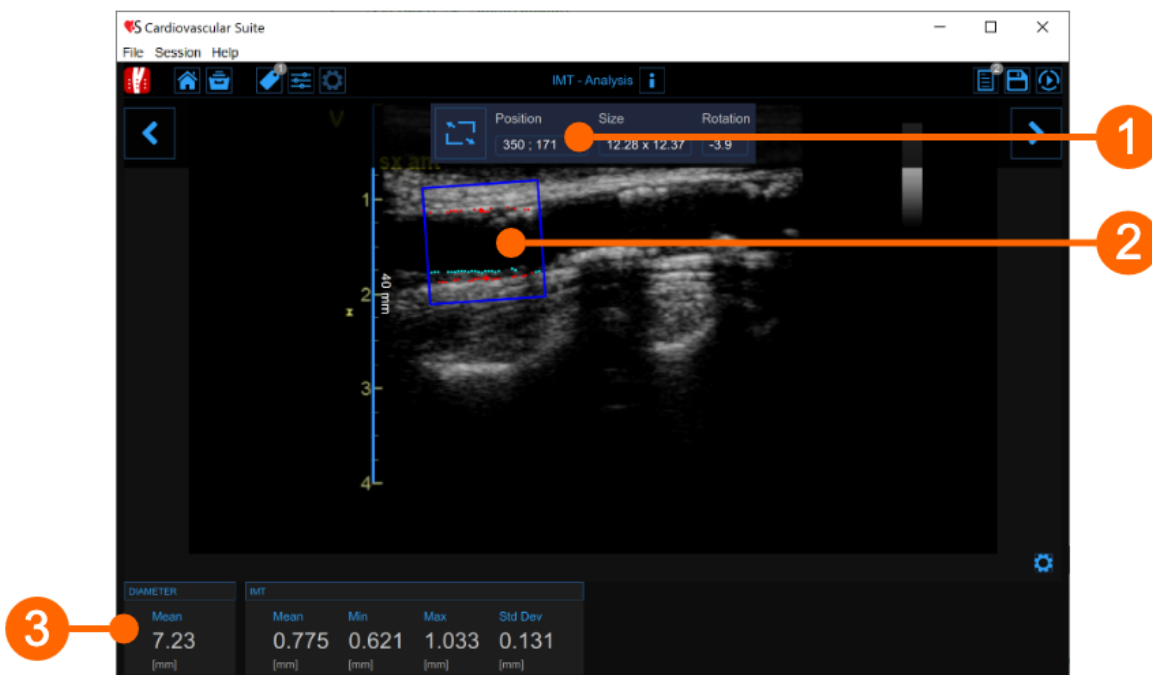

The IMT analysis window contains the following components:

1 Setup panel

The Set ROI  button is used to set the ROI.

The numeric display "Position" shows the position, in pixels, of the ROI (central point). The numeric display "Size" shows the size (width x height), in pixels, of the ROI. The numeric display "Rotation" shows the degree of rotation of the ROI (degrees).

NOTE: if you click in the value fields, you are allowed to manually enter the ROI position, the size, and the rotation in the editable fields (if you already know the values). The click the Save button to enter the values.




2 ROI

The Region of Interest (ROI) is the portion of the image where both the diameter and the IMT are calculated. The points of the Lumen-Intima interface and the Media-Adventitia interface are displayed within the ROI in cyan and red color respectively. The ROI can be moved, resized, and/or rotated. Each time you change the position, size and/or inclination of the ROI, the analysis is re-initialized.


Draw a new ROI:

You can manually draw the diameter ROI with the desired size and position. If the image is already calibrated, you can also more quickly draw a diameter ROI with the default sizes set in [Carotid Studio settings](#) (a star in the Set ROI button will indicate that the default ROI can be drawn). The default ROI is also automatically rotated so to be parallel to the carotid artery.

default ROI drawing


- Click on the Set ROI  button in the Setup panel (the button remains active)
- Click in the video window in the center of the carotid artery.
- A ROI of the default ROI sizes will be automatically initialized.

manual drawing

- Click on the Set ROI  button in the Setup panel (the button remains active).
- Click inside the video window and drag until the ROI is complete (the size of the ROI is shown in the Setup panel and graphically within the ROI).
- When you release the mouse, the analysis is initialized.

Rotate the ROI:

- Click immediately outside the ROI (a special cursor that indicates a rotation is shown)
- Hold inside the ROI, drag the rectangle by rotating it to the desired angle

 As an alternative, you can modify the position of the ROI by typing the value in the Setup Panel.

Resize the ROI:

- Click on one of the sides or one of the corners of the ROI.
- Drag to change the size of the ROI.

i As an alternative, you can modify the size of the ROI by typing the value in the Setup Panel.

Move the ROI:

- Click and hold inside the ROI.
- Drag the ROI to the location of interest.

i As an alternative, you can modify the position of the ROI by typing the value in the Setup Panel.


Re-initialize the ROI:

- Double click inside the Diameter ROI to re-initialize the position and the rotation of the ROI.

3 Data panel

This panel contains the computed values. In particular, it shows the mean diameter value and minimum, maximum, mean, and standard deviation of IMT.

10.3.2 Plaque analysis

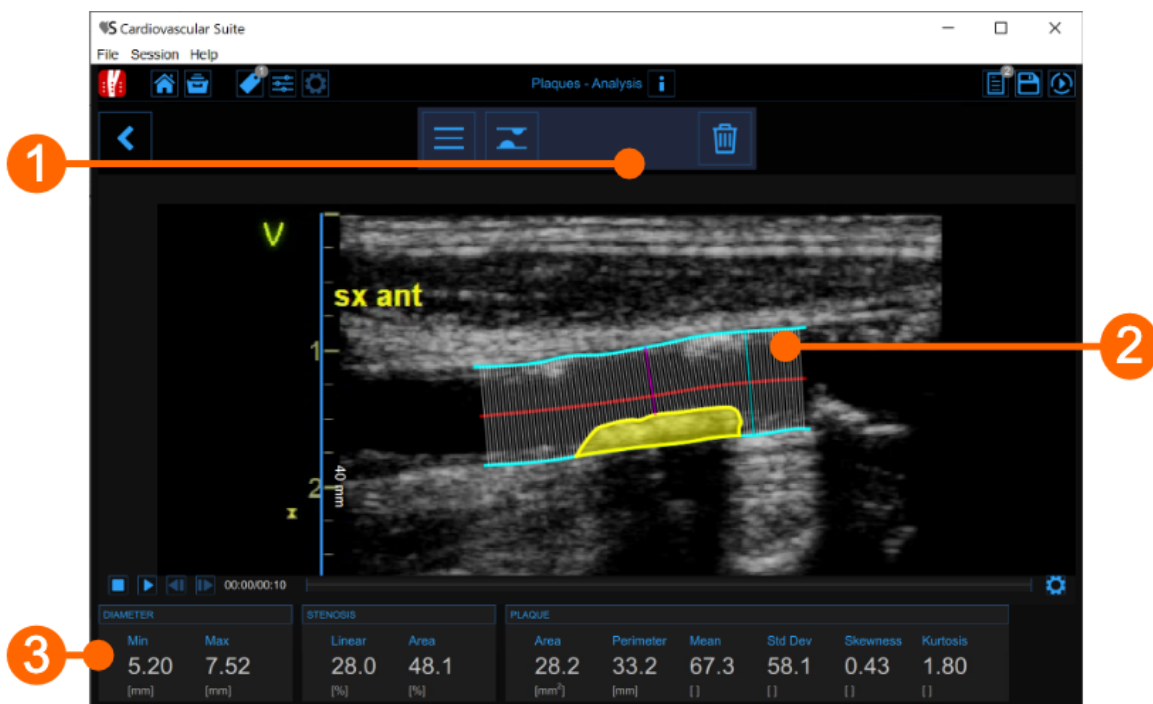

The plaque analysis window contains the following components:

1. Setup panel


It contains the controls for tracing of the vessel borders, drawing a plaque and delete it.


2. Plaque analysis tool


The Trace borders



button is used to manually trace the borders of the vessel. The user has to trace point-by-point the vessel edges and the software interpolates them. It is possible to modify the points by dragging them, as shown in the following picture.

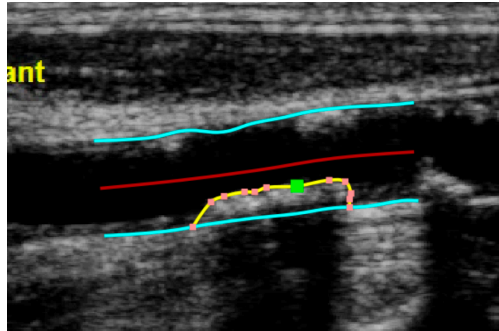

After the two borders are traced, the software automatically compute the minimum and maximum values of the diameter and the linear and circular values of the stenosis. The Draw plaque  button is used to manually draw the profile of a plaque. The user has to trace point-by-point the plaque profile and the software interpolates them. Also in this case, it is possible to modify the points by dragging them and to delete a plaque, as shown in the following picture.

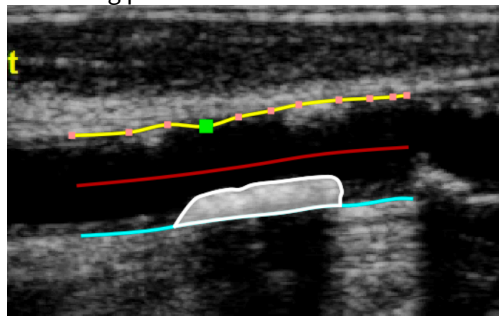


After the plaque is drawn, the software automatically computes its area, perimeter, and the mean, standard deviation, skewness, and kurtosis of its grey level.

3. Data panel


This panel contains the computed values. In particular, it shows the minimum and maximum values of the diameter and the linear and circular values of the stenosis. In addition, if a plaque has been drawn, it also displays its area and perimeter, and the mean, standard deviation, skewness, and kurtosis value of its grey level.

10.3.3 Tags

The Tags Management  button opens a panel that allows to associate a tag to the document, or create a new tag. Carotid studio can use two types of tags:


1. System tags, which are already defined in Cardiovascular Suite. System tags are used to specify which segment of the Carotid artery is analysed, and are necessary to include the document data in the study report. Only one system tag can be associated to a document.
2. Custom tags, which are defined by the user and are used to better identify a document.

Custom tags can also be managed through the Tags management into the Archive.

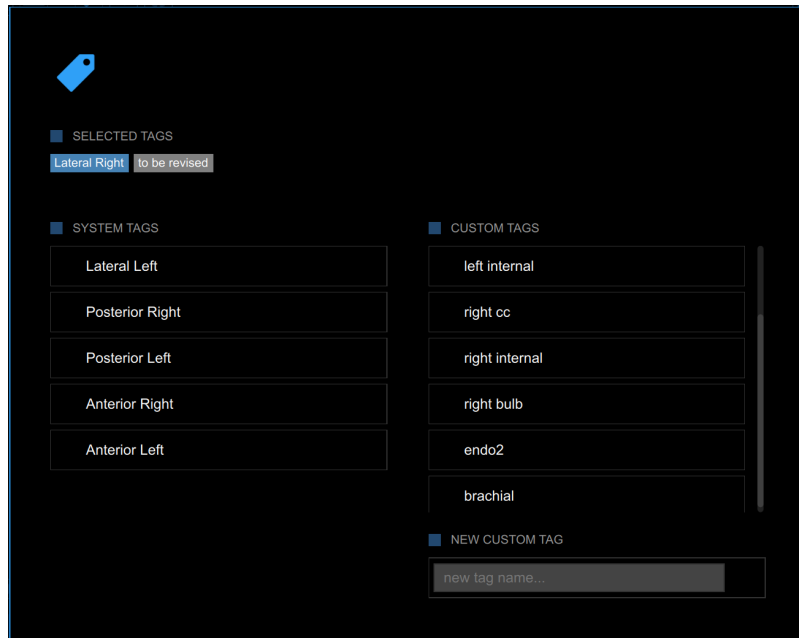


The selected tags are visible in a special area of the Analysis window. The tags area can be moved by right clicking and dragging.

10.3.4 Presets

The preset management  button opens the preset management panel that allows to manage presets. In particular, it allows to remember the settings of:

- B-mode image calibration
- B-mode image ROI (size, position, and rotation)

A preset can be saved and reused for following studies.

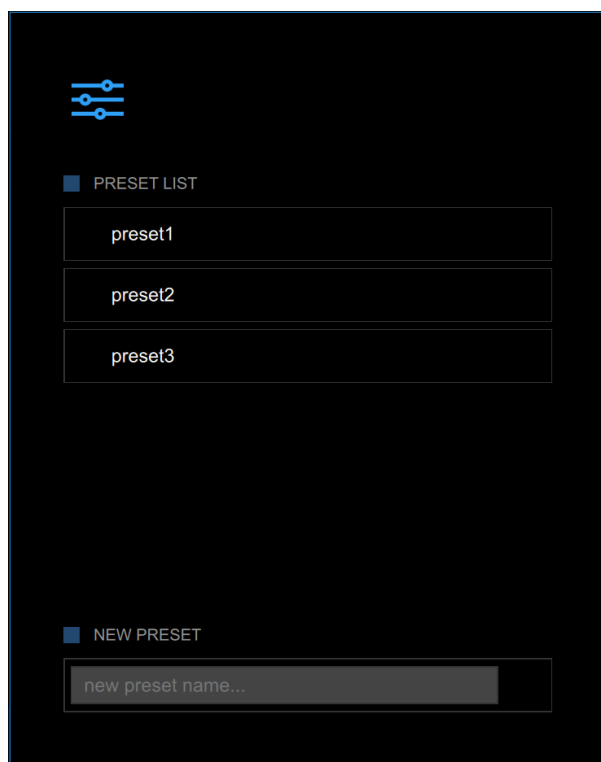



10.4 Calibrate the B-mode image


The calibration of the images must be done before starting a new examination because it is necessary to provide information about the size of the image generated by ultrasound system. The calibration factor changes depending on the settings of your ultrasound machine. You should check the calibration at each new examination.

⚠ CAUTION: the lack of calibration can generate a software malfunction.



- Locate, in ultrasound image, a range of known distance (30 mm. in the example of figure).
- In the B-mode setup panel, select from the drop-down menu, the distance specified above.
- In the B-mode setup panel, click on the Set B-Mode Calibration  button (button remains active).
- Draw a line on the image corresponding to the known distance: click on one end and drag the mouse to the other extreme (press the Shift key or CTRL Shift keys on your keyboard if you want the line to be not vertical or horizontal).

 For DICOM files, when present, the B-mode calibration is obtained automatically by the file metadata (see [Settings](#)). You can anyhow modify the calibration value.

 You can directly type the calibration value in the Calibration factor field of the B-mode setup panel if you already know the value.

10.5 Cineloop study review



The Review window shows the result of the analysis and allows you to remove piece of data that are considered to be "outliers". In the Review window you can review both the images and the result of the analysis and decide to remove the data that were generated in this time interval.


The Review window contains the following components:


1. [Top bar](#)
2. [Diameter chart](#)
3. [IMT chart](#)


4. [Video window](#)
5. [Results panel](#)



10.5.1 Top bar


The top bar contains some essential information for the navigation.

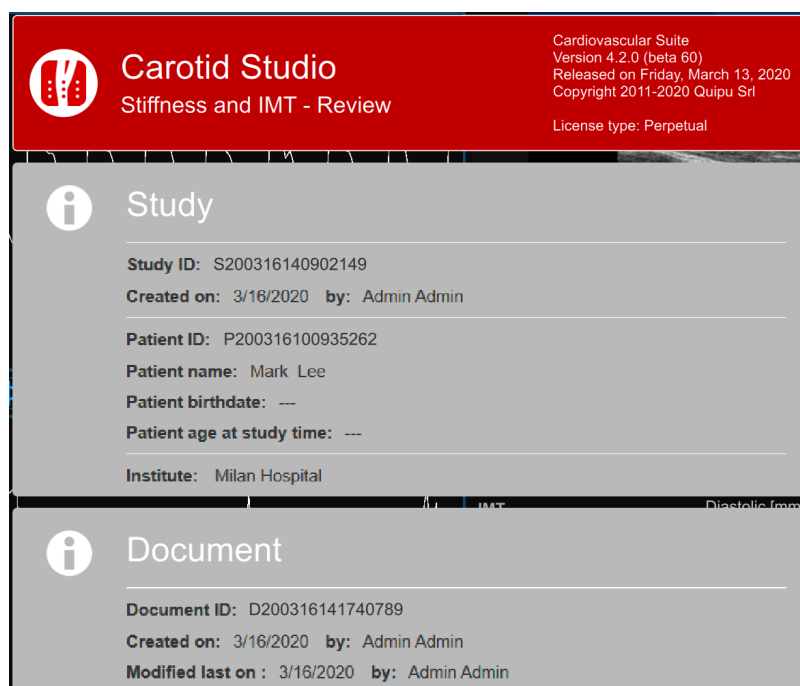



The Carotid Studio button  shows a panel containing some information about Cardiovascular Suite, about the current study and the current document. Regarding the study, the study ID is displayed together with information about the patient and the institute. In addition, info regarding the current document are provided. Information about the software, such as version and type of license, are shown in the upper part of the panel.





The home button  closes the Carotid Studio application and returns to the home screen of Cardiovascular Suite. The back button  closes the Carotid Studio application and comes back to the Archive.


The Tags Management button  opens a panel (see the following picture) that allows to create a new tag and associate it or an existing tag to the document. Tags can be managed through the [Tags management](#) into the Archive.

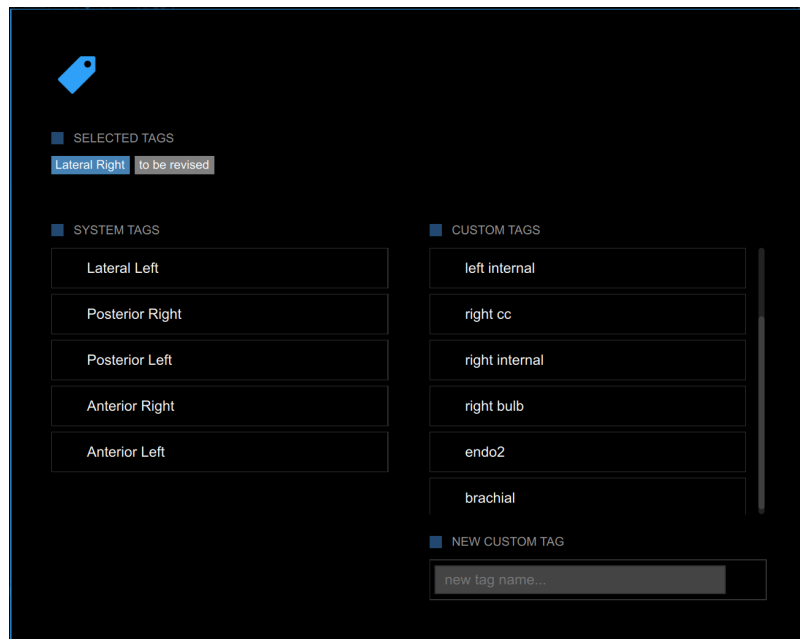


The Notes  button can be used to enter a note in the document.

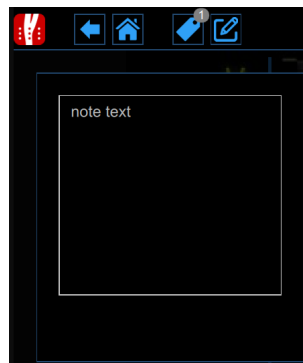

The Save  button is used to save your changes to the document, once you have edited the data.


The Delete the document  button is used to delete the current document.

The Export  button is used to export your data. You can export the Document Results and the Document Data.

The **Document Results** contains all the results of the analysis and all the information about the study, the document and the patient.


The **Document Data** contains all the Document Results, a list of the Diameter and the IMT values computed at each frame.

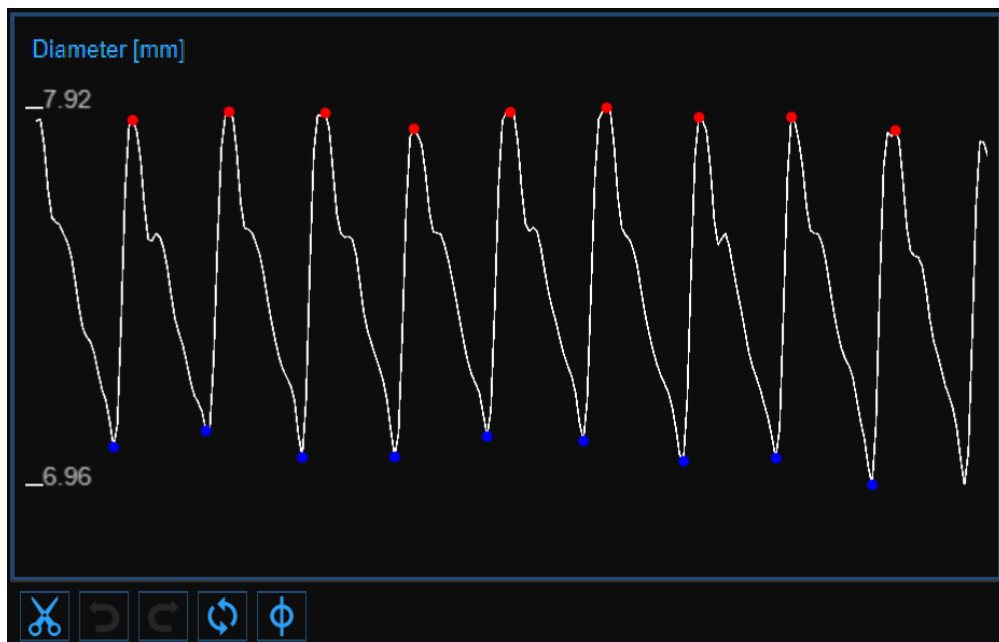


10.5.2 Diameter chart





The chart shows the trend of the diameter. The buttons on the bottom can be used for editing the chart and removing the outliers.


10.5.2.1 Remove the outliers

- Click on the Cut  button. The heart cycle will be highlighted in the diameter chart.
- Click on the cardiac cycles you want to remove.
- Once you have removed the outliers, the data on the [Results panel](#) will be automatically updated.

You can use the undo  and redo  buttons to cancel and restore your changes. The Restore  button cancels all your changes and restore original data.


 Click on the Save  button in the Top Bar to save your changes to the document.

10.5.2.2 Graph cursors

As shown in the following figure, the Cursor  button **(1)** activates a cursor **(2)** on the Diameter chart that shows the current time position on the graph according to the images shown in the [Video window](#). The coordinates (diameter value in millimeters and time value in the format *minutes:seconds.milliseconds*) of the cursor are dynamically updated and shown in **(3)**. When the Cursor button is active, it is also possible to know the coordinates of an exact point in the graph; it is only needed to hover over the chart and a second cursor **(4)** is displayed. It follows the mouse movements and the exact coordinates of the point are shown in the label **(5)** (diameter value is expressed in millimeters and the time value has the format *minutes:seconds.milliseconds*).



10.5.3 IMT chart

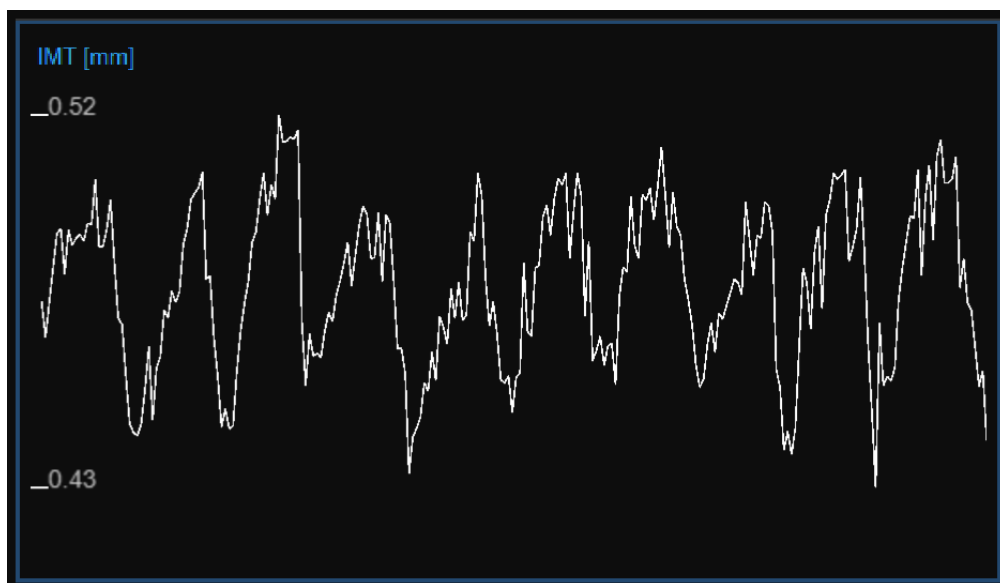




The chart shows the trend of the IMT. The buttons at the top can be used for editing the chart and removing the outliers.

10.5.3.1 Remove the outliers


- Click on the Cut  button.

- In the IMT chart, click on one of the two extremes of the range to be deleted.
- Drag the mouse horizontally to the other extreme of the range to be deleted.
- Once you have removed the outliers, the data on the [Results panel](#) will be automatically updated.

You can use the undo  and redo  buttons to cancel and restore your changes. The restore  button cancels all your changes and restore original data.


Note: Click on the Save  button in the [Top bar](#) to save your changes to the document.

10.5.3.2 Graph cursors

As shown in the following figure, the Cursor  button **(1)** activates a cursor **(2)** on the IMT chart that shows the current time position on the graph according to the images shown in the [Video window](#). The coordinates (IMT value in millimeters and time value in the format *minutes:seconds.milliseconds*) of the cursor are dynamically updated and shown in **(3)**. When the Cursor button is active, it is also possible to know the coordinates of an exact point in the graph; it is only needed to hover over the chart and a second cursor **(4)** is displayed. It follows the mouse movements and the exact coordinates of the point are shown in the label **(5)** (IMT value is expressed in millimeters and the time value has the format *minutes:seconds.milliseconds*).




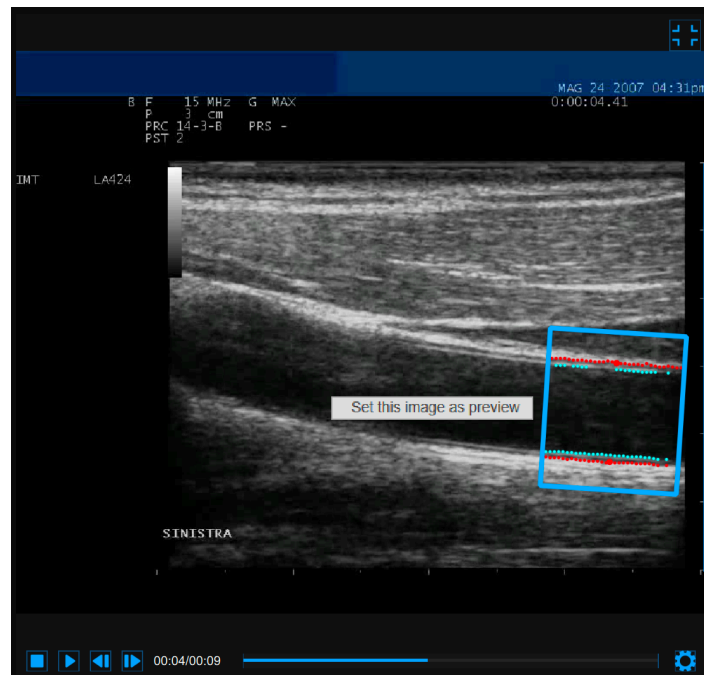
10.5.4 Video window

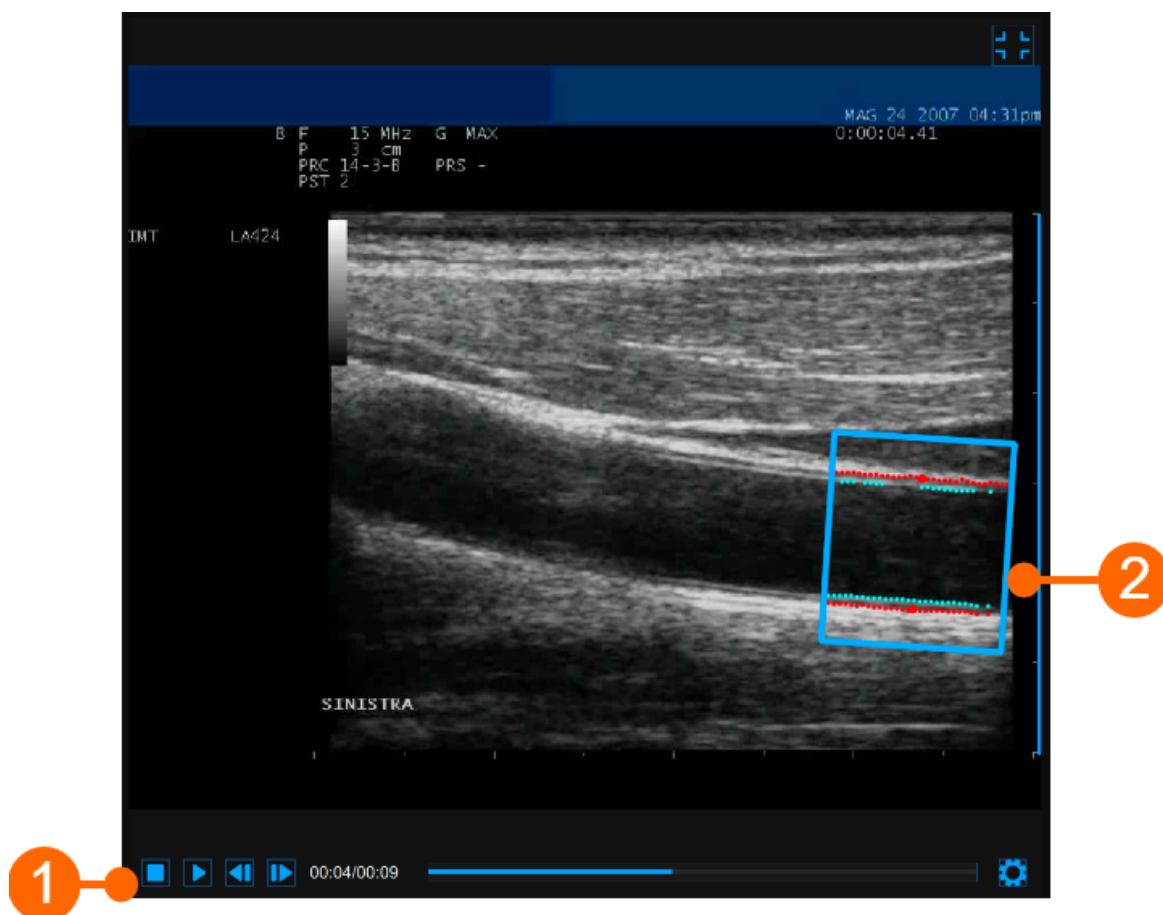

The video window shows the video signal from your ultrasound system. The points of the Lumen-Intima interface and the Media-Adventitia interface are displayed within the ROI (2) in cyan color.


The video control bar (1) is located at the bottom of the window.

If you want to expand the video window, you have to click on the Enlarge  button.



- ✓ If you perform right click on the video window and click on "Set this image as preview" the current frame will be saved and displayed in the Documents Table as document preview (see [Studies management](#)).

10.5.5 Results panel

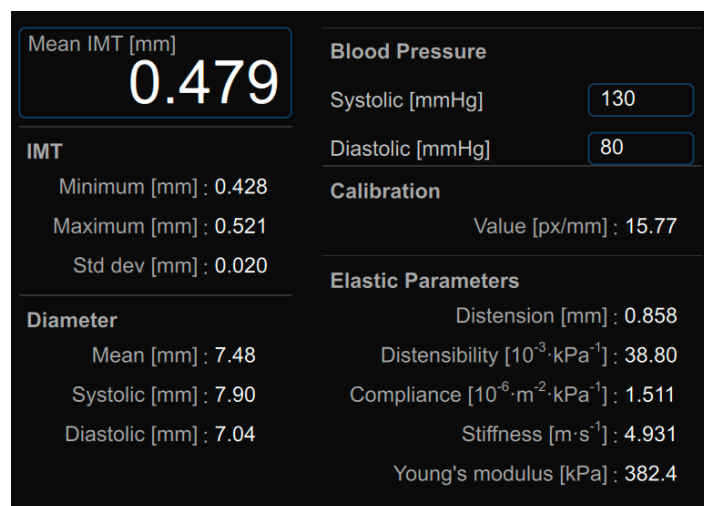

The panel shows the results of the analysis. The following data are displayed:

- **Calibration value [px/mm]**
- **Mean IMT [mm]:** Intima Media Thickness. It is computed as an average value of the data present in the [IMT chart](#).
- **Minimum IMT [mm]:** minimum value of Intima Media Thickness. It is computed on the data present in the [IMT chart](#).

- **Maximum IMT [mm]:** maximum value of Intima Media Thickness. It is computed on the data present in the [IMT chart](#).
- **Std. dev IMT [mm]:** standard deviation of Intima Media Thickness. It is computed on the data present in the [IMT chart](#).
- **Mean diameter [mm]:** value of the average diameter. It is computed as an average value of the diameter data present in the [Diameter chart](#).
- **Systolic diameter [mm]:** value of the diameter in systole. It is computed as an average value of the systolic diameters present in the [Diameter chart](#).
- **Diastolic diameter [mm]:** value of the diameter in diastole. It is computed as an average value of the diastolic diameters present in the [Diameter chart](#).
- **Blood pressure [mmHg]:** diastolic pressure and systolic pressure.
- **Distension [mm]:** stroke change in diameter.

$$Distension = \Delta D = D_s - D_d$$

- **Compliance [$10^{-6} \cdot m^2 \cdot kPa^{-1}$]:** absolute change in lumen area for a given pressure change.

$$Compliance = \frac{\Delta A}{\Delta P} = \frac{\pi}{4} \cdot \frac{D_s^2 - D_d^2}{P_s - P_d}$$

- **Distensibility [$10^{-3} \cdot kPa^{-1}$]:** relative change in lumen area during systole for a given pressure change.

$$Distensibility = \frac{1}{A_d} \cdot \frac{\Delta A}{\Delta P} = \frac{1}{D_d^2} \cdot \frac{D_s^2 - D_d^2}{P_s - P_d}$$

- **Carotid Stiffness [$m \cdot s^{-1}$]:** Stiffness value computed by Bramwell-Hill equation.

$$Stiffness = \frac{1}{\sqrt{\rho \cdot Distensibility}} = \sqrt{\frac{A_d \cdot \Delta P}{\rho \cdot \Delta A}} = \sqrt{\frac{D_d^2 \cdot (P_s - P_d)}{\rho \cdot (D_s^2 - D_d^2)}}$$

- **Young's elastic modulus [kPa]:**

$$Young's Modulus = \frac{3}{Distensibility} \cdot \left(1 + \frac{A_d}{WCSA}\right)$$

where:

D_e = External Diameter (between the media-adventitia interfaces) measured in diastole.

D_i = Internal Diameter (between the lumen-intima interfaces) measured in diastole.

D_s = Systolic Diameter (external).

D_d = Diastolic Diameter (external), $D_d = D_e$

WCSA = Wall Cross Section Area

$$WCSA = \frac{\pi}{4} \cdot (D_e^2 - D_i^2)$$

ΔA = Stroke change in lumen area.

$$\Delta A = \frac{\pi}{4} \cdot (D_s^2 - D_d^2)$$

A_d = Diastolic Area.

$$A_d = \frac{\pi}{4} \cdot D_d^2$$

P_s = Systolic Pressure.

P_d = Diastolic Pressure.

$\Delta P = P^s - P^d$

ρ = Blood density: is assumed to be constant and equal to 1.06 g/cm³.


These data can be exported in the Document Data. See [here](#) for export details.

10.6 Single image study review

Carotid Studio single image modality, depending on the performed analysis, generates two different types of documents:

1. [IMT document](#)
2. [Plaque document](#)


10.6.1 IMT review

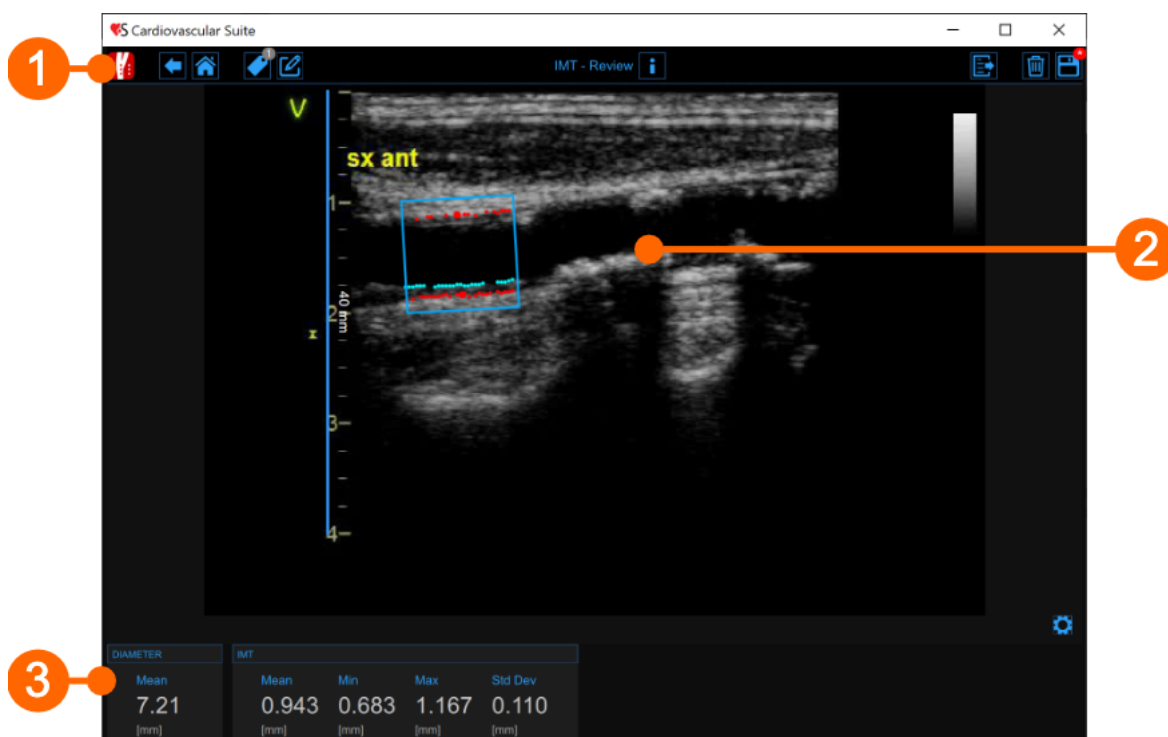




The Review window contains the following components:


1. Top bar


The top bar contains some essential information for the navigation.

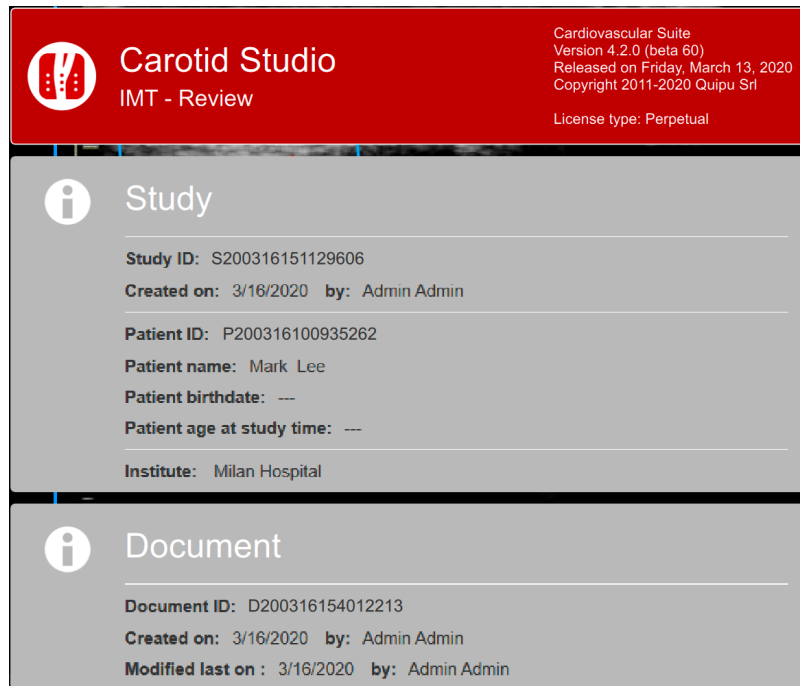
The Carotid Studio button  shows a panel containing some information about Cardiovascular Suite, about the current study and the current document. Regarding the study, the study ID is displayed together with information about the patient and the institute. In addition, info regarding the current document are provided. Information about the software, such as version and type of license, are shown in the upper part of the panel.





The home button  closes the Carotid Studio application and returns to the home screen of Cardiovascular Suite. The Back  button closes Carotid Studio and goes back to the Archive.


The Tags Management button  opens a panel (see the following picture) that allows to create a new tag and associate it or an existing tag to the document. Tags can be managed through the [Tags management](#) into the Archive.

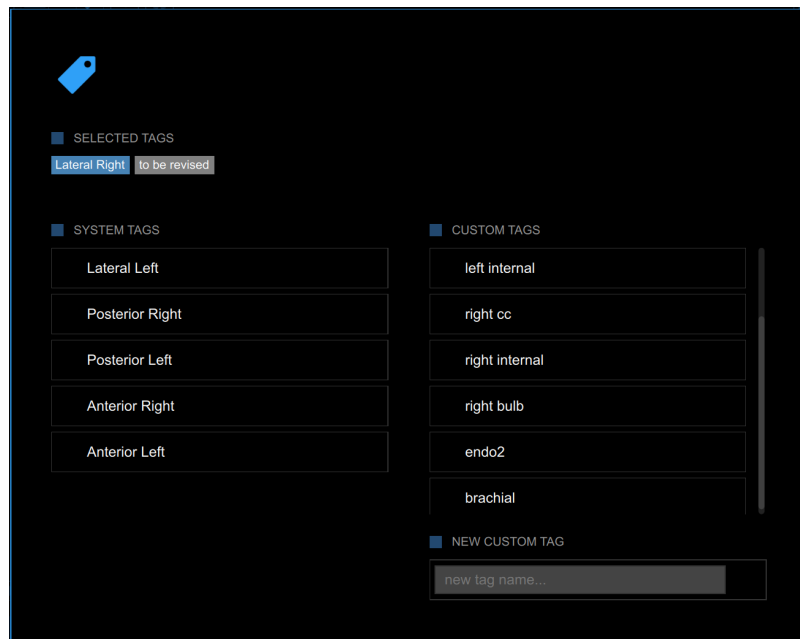


The Notes  button can be used to enter a note in the document.

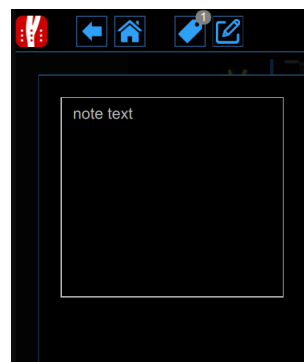

The Save  button is used to save your changes to the document, once you have edited the data.

The Delete the document  button is used to delete the current document.

The Export  button is used to export your data. You can export the **Document Results** that contains all the results of the analysis and all the information about the study, the document and the patient.

2. Image window

The image window shows the media file that has been analysed. It shows also the ROI and the calibration line used.


3. Results panel

The panel shows the results of the analysis. The following data are displayed:

- **Mean diameter [mm]:** value of the average diameter. It is computed as an average value of the data present in the ROI.
- **Mean IMT [mm]:** Intima Media Thickness. It is computed as an average value of the data present in the ROI.

- **Minimum IMT [mm]:** minimum value of Intima Media Thickness. It is computed on the data present in the ROI.
- **Maximum IMT [mm]:** maximum value of Intima Media Thickness. It is computed on the data present in the ROI.
- **Std. dev IMT [mm]:** standard deviation of Intima Media Thickness. It is computed on the data present in the ROI.


10.6.2 Plaque review

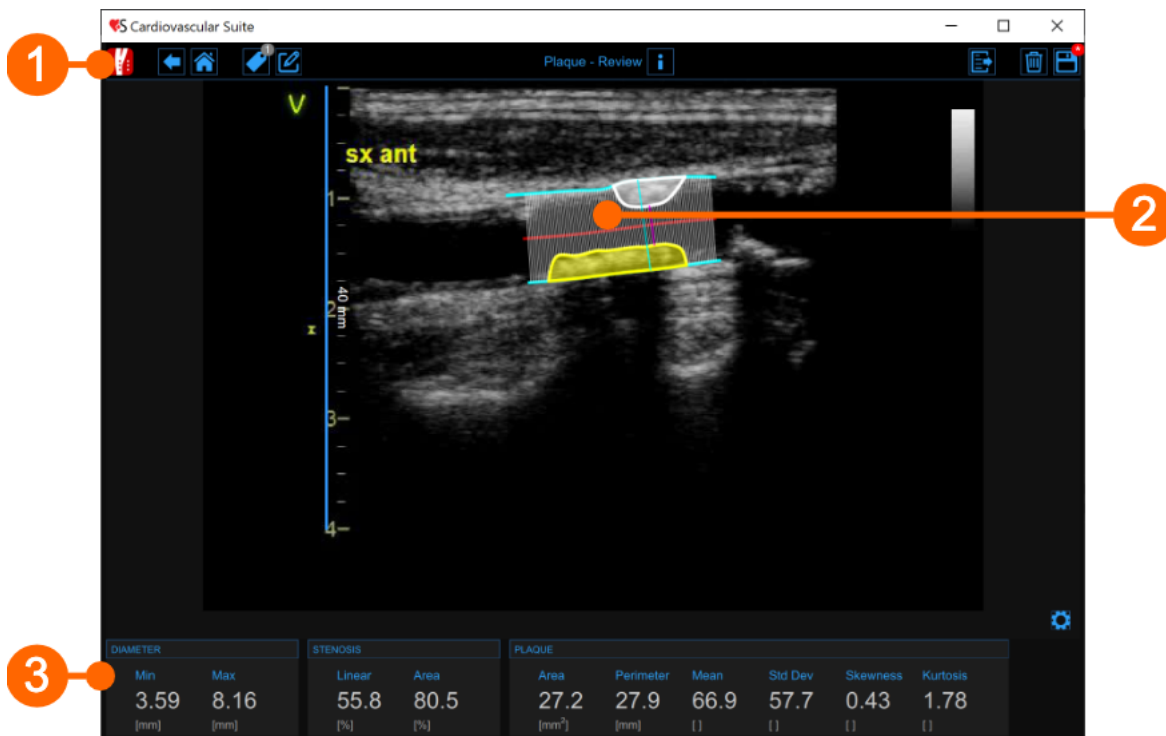


The Review window contains the following components:

1. Top bar

The top bar contains some essential information for the navigation.

The Carotid Studio button  shows a panel containing some information about Cardiovascular Suite, about the current study and the current document. Regarding the study, the study ID is displayed together with information about the patient and the institute. In addition, info regarding the current document are provided. Information about the software, such as version and type of license, are shown in the upper part of the panel.



Carotid Studio

Plaque - Review


Cardiovascular Suite

Version 4.2.0 (beta 60)

Released on Friday, March 13, 2020

Copyright 2011-2020 Quipu Srl

License type: Perpetual



Study

Study ID: S200316151129606

Created on: 3/16/2020 by: Admin Admin


Patient ID: P200316100935262

Patient name: Mark Lee

Patient birthdate: ---

Patient age at study time: ---

Institute: Milan Hospital






Document


Document ID: D200316154020555

Created on: 3/16/2020 by: Admin Admin

Modified last on : 3/16/2020 by: Admin Admin

The Home  button closes the Carotid Studio application and returns to the home screen of Cardiovascular Suite. The Back  button closes Carotid Studio and goes back to the Archive.

The Tags Management  button opens a panel (see the following picture) that allows to create a new tag and associate it or an existing tag to the document. Tags can be managed through the [Tags management](#) into the Archive.



SELECTED TAGS

Lateral Right to be revised

SYSTEM TAGS

Lateral Left

Posterior Right

Posterior Left

Anterior Right

Anterior Left

CUSTOM TAGS

left internal

right cc

right internal


right bulb


endo2

brachial


NEW CUSTOM TAG


new tag name...

The Notes  button can be used to enter a note in the document.

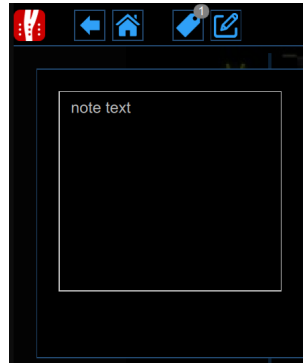

The Save  button is used to save your changes to the document, once you have edited the data.

The Delete the document  button is used to delete the current document.

The Export  button is used to export your data. You can export the **Document Results** that contains all the results of the analysis and all the information about the study, the document and the patient.

2. Media window

The media window shows the media file that has been analysed. It shows the plaque analysis tool and the calibration line used. It displays also the drawn plaques.

3. Results panel


The panel shows the results of the analysis. The following data are displayed:

- **Min diameter [mm]**: minimum value of the diameter.
- **Max diameter [mm]**: maximum value of the diameter.
- **Linear stenosis [%]**: percent of linear stenosi (computed on the diameter)
- **Area stenosis [%]**: percent of area stenosi (computed on the cross section area)
- **Plaque area [mm²]**: area of the plaque
- **Plaque perimeter [mm]**: perimeter of the plaque
- **Plaque mean []**: mean value of the grey levels in the plaque
- **Plaque std dev []**: standard deviation of the grey levels in the plaque
- **Plaque skewness []**: skewness of the grey levels in the plaque
- **Plaque kurtosis []**: kurtosis of the grey levels in the plaque

10.7 Study report

The study report summarises the results of the documents of the study.

The report includes only the study documents that have a system tag. This is because the tag is necessary to identify the scan view (lateral, posterior or anterior) and the carotid artery (left or right).

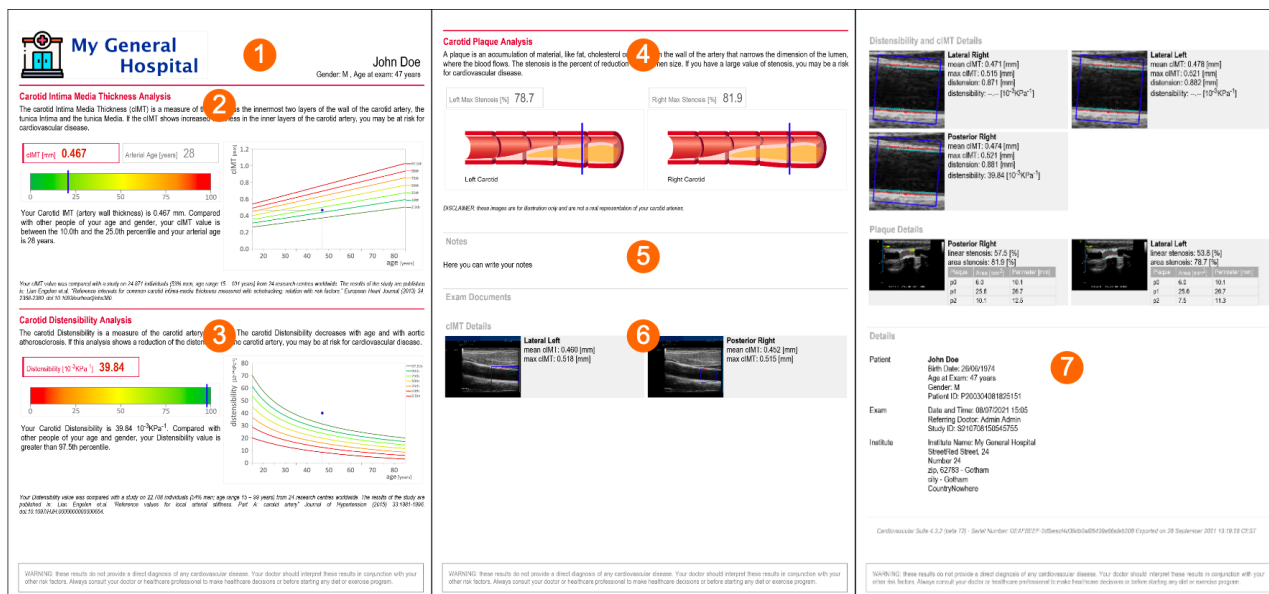

The report has the following sections:

1. Header
2. Carotid Intima Media Thickness Analysis
3. Carotid Distensibility Analysis
4. Carotid Plaque Analysis
5. Notes
6. Exam documents
7. Details

10.7.1 Header

The header contains the patient Name, gender and age, and the logo of the institute. The logo can be set in [Institute management](#).

10.7.2 Carotid Intima Media Thickness Analysis

This section reports a **mean value** of carotid IMT that is obtained as the average of the IMT values contained in the documents included in the report. Both documents of "IMT" type and "Stiffness and IMT" type are used to compute this value. The carotid IMT value is compared with reference values published in Lian Engelen et.al. "Reference intervals for common carotid intima media thickness measured with echotracking: relation with risk factors." European Heart Journal (2013) 34, 2368-2380. The percentile of the carotid IMT value is reported. The arterial age value, which is calculated as the value at which the IMT value corresponds to the 50-th percentile of the reference population, is also reported.

This section will be present in the report only if data are available, i.e. if the report includes documents of "IMT" type and/or "Stiffness and IMT" type.

10.7.3 Carotid Distensibility Analysis

This section reports a **mean value** of carotid distensibility that is obtained as the average of the distensibility values contained in the documents included in the report. Documents of "Stiffness and IMT" type are used to compute this value. The carotid distensibility value is compared with reference values published in Lian Engelen et.al. "Reference

values for local arterial stiffness. Part A: carotid artery" J Hypertension 2015 Oct. 33(10):1981-96. The percentile of the carotid distensibility value is reported.

This section will be present in the report only if data are available, i.e. if the report includes documents of "Stiffness and IMT" type, where the distensibility is computed.

10.7.4 Carotid Plaque Analysis

This section reports the maximum value of the [linear stenosis](#) for both the left and the right carotid. Documents of "Plaque" type are used to compute this value.

This section will be present in the report only if data are available, i.e. if the report includes documents of "Plaque" type.

10.7.5 Notes

This section contains the study notes that can be set in the Study view window (see [Studies management](#)).

10.7.6 Exam documents

This section contains a summary of the results of all the documents included in the report.

Details

This section contains details on the Patient, Study and Institute data.


11 FMD Studio

FMD Studio is a software for the measurement of the Flow-Mediated Dilation (FMD) or other general Vasodilation of the brachial artery.

11.1 Create a new study


When you start FMD Studio, a procedure guides you in the creation of a new study. The steps are:


11.1.1 Select the source

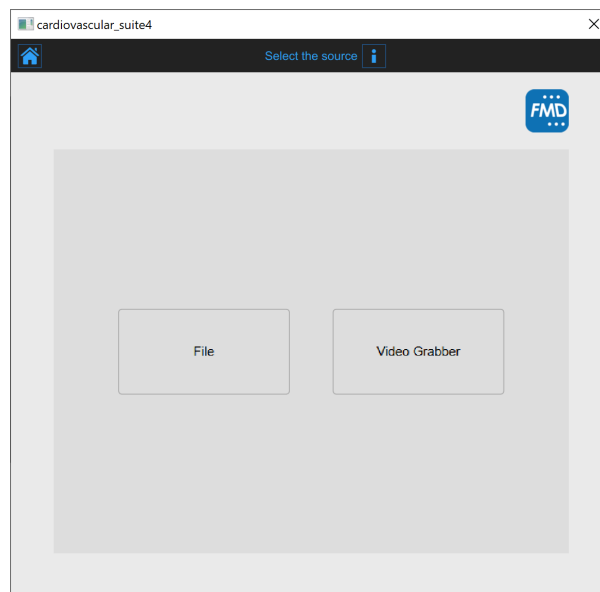


In this tab, you can select the study video source. FMD Studio processes video sources and can work in offline modality by processing a Video File or a DICOM File or in real time by processing images directly coming from the ultrasound equipment thanks to a video converter.



11.1.2 Select the patient

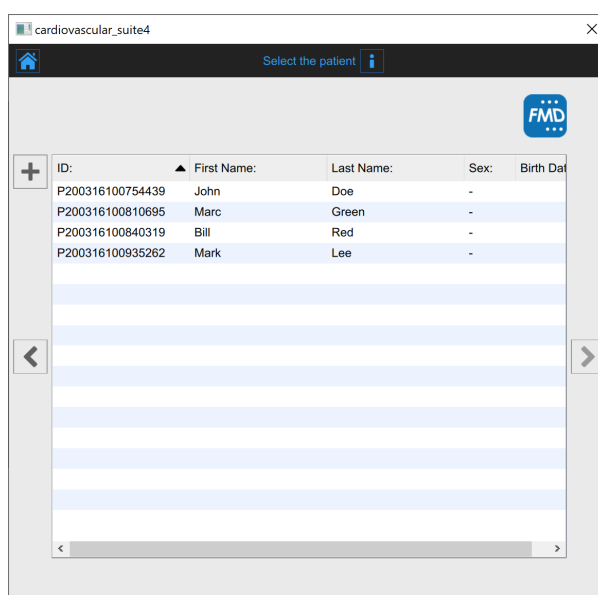
 For DICOM files, the patient data are obtained by the file metadata and this window is skipped (see [Settings](#)). You can anyhow edit the patient data from the Review window.



ID:	First Name:	Last Name:	Sex:	Birth Date:
P200316100754439	John	Doe	-	
P200316100810695	Marc	Green	-	
P200316100840319	Bill	Red	-	
P200316100935262	Mark	Lee	-	

In this tab, you can select the patient among the ones already present in the [Archive](#). Select the patient and click on the Next  button (you can simply double-click on the patient to proceed).


If you want to create a new patient, click on the Add New Patient  button. In the Add new patient frame, enter the patient data. The only mandatory field is the patient ID. If you don't enter patient ID a random value is automatically proposed. Click on the Save  button to save the patient data.

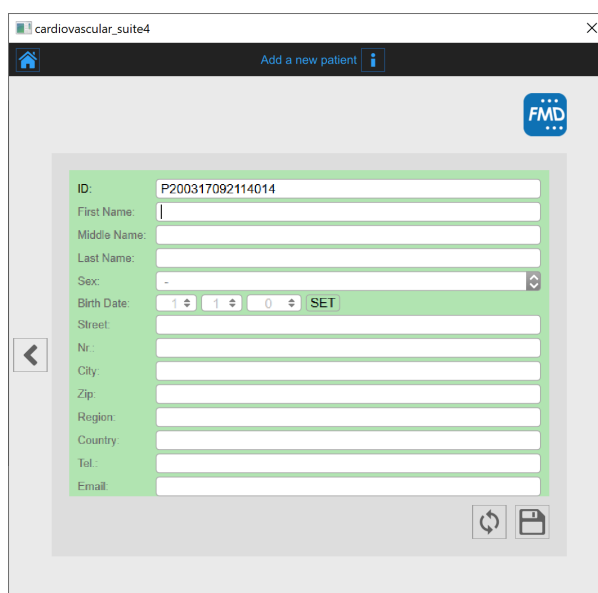




ID:	P200317092114014
First Name:	
Middle Name:	
Last Name:	
Sex:	-
Birth Date:	1 1 0 SET
Street:	
Nr.:	
City:	
Zip:	
Region:	
Country:	
Tel.:	
Email:	


11.1.3 Select the institute

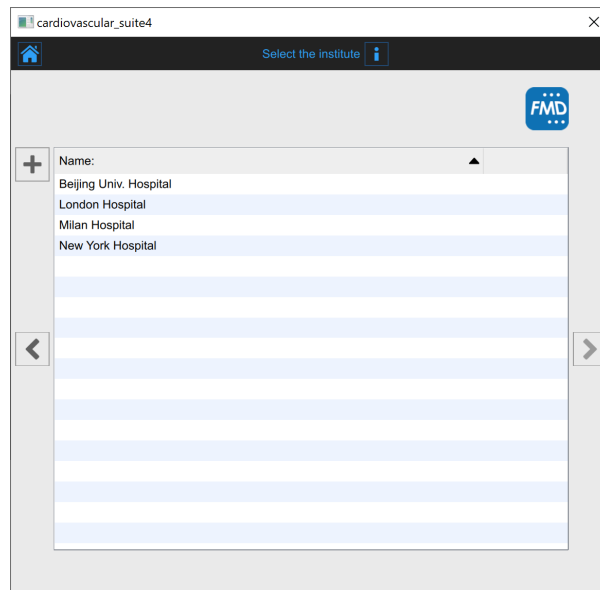i If it is the first time you create a study, after selecting the patient you will also need to select the institute. If you have already created at least one study, the software remembers the institute used for the previous study and after selecting the patient shows you automatically the final review (where you can still make changes before starting the new study).






In this tab, you can select the institute among the ones already present in the [Archive](#). Select the institute and click on the Next  button (you can simply double-click on the institute to proceed).

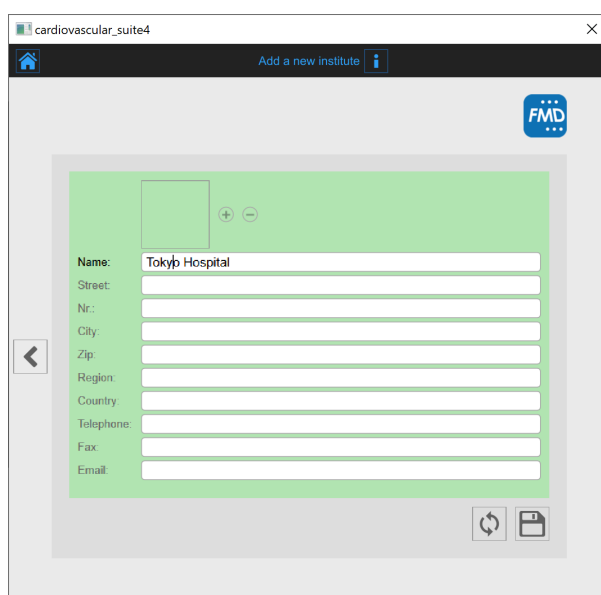
If you want to create a new institute, click on the Add New Institute  button. In the Add new institute frame, enter the institute data. The only mandatory field is the Name. Click on the Save  button to save the institute data.




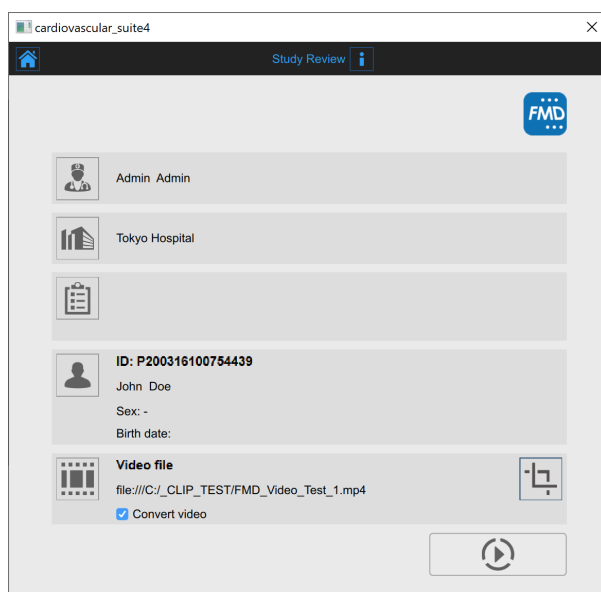

11.1.4 Review





In this tab you can review your selection (you can also change Patient  and Institute  by clicking on their buttons). It is possible also to change the selected source for this study by clicking on the icon that represents the source.

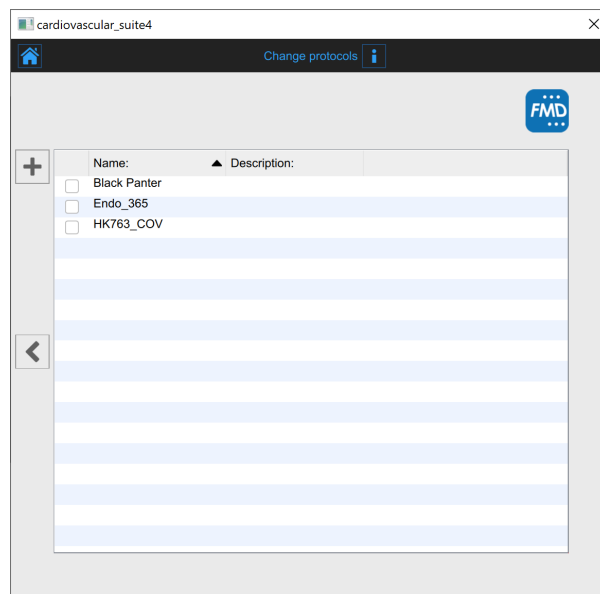
Here, the user has the possibility to associate the study to one or more existing protocols, by clicking on the protocols icon .




In the Protocols tab, you can associate the study to one or more than one protocols already present in the Archive. Put a tick on the protocol you want to associate the study with. If you want to create a new protocol, click of the Add New protocol  button. In the Add new institute frame, enter the protocol data. The mandatory field (Name) is in red until you have filled in the Name blank. Click on the Save  button to save the protocol data.

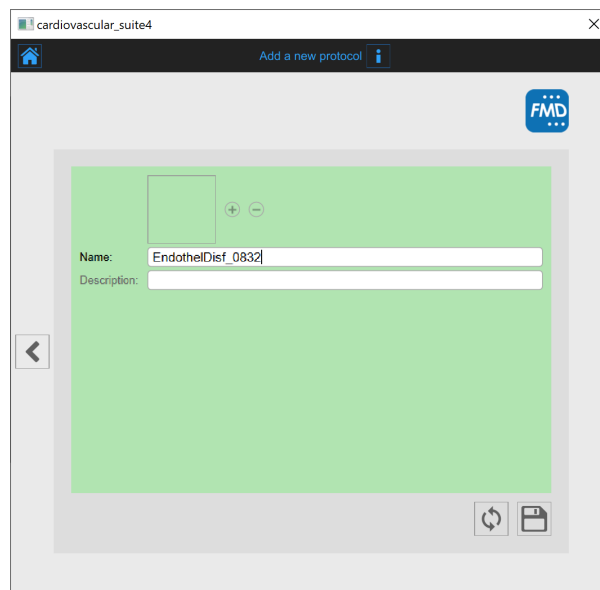



Click on the Previous  button to go back to the review window.


 If in the [Settings manager](#) the option "Remember last used protocols" is checked, the study will be associated by default with the last used protocols.


In addition, if you have chosen a video file as source, in the review window, it is possible to convert the video file to be optimized for the analysis with Carotid Studio. This operation may take few minutes.

 The default value of the "Convert video" checkbox is set by the "Convert video by default" option in the [Settings manager](#).

You can also crop the images by clicking the Crop  button in the source panel. In this case, a new window opens; it is possible to select a region to be used for the analysis. Click on the Confirm  button after you have drawn the region.



Click on the Start the Study  button to proceed. A progress bar, as shown in the following picture, will show you the progression of the study creation.

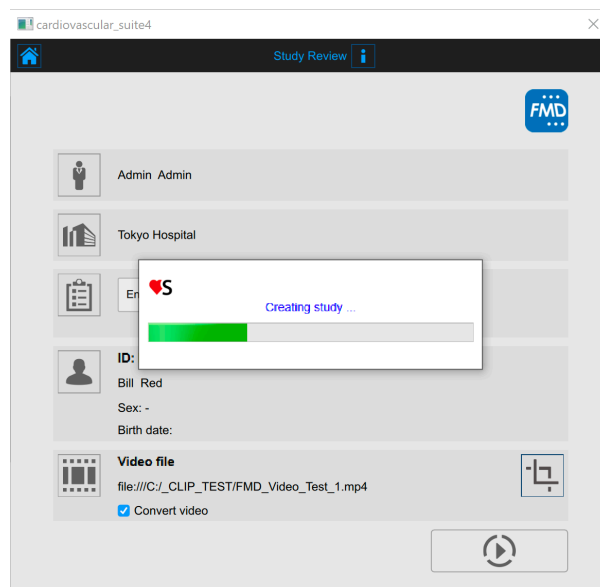

11.2 Analysis




The Analysis window contains the following components:


1. Top bar
2. Video window
3. Mean diameter chart
4. Shear rate chart
5. Instantaneous diameter chart
6. Setup panel
7. Tags


11.2.1 Top bar


The top bar contains some essential information for the navigation.



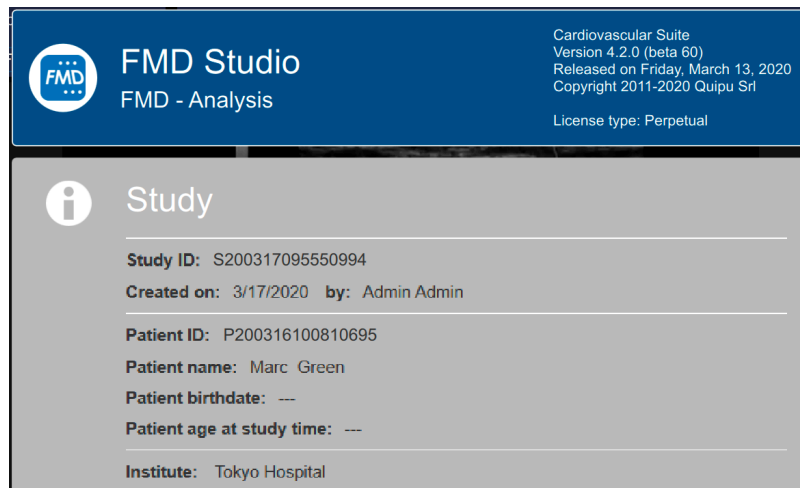

The FMD Studio  button shows a panel containing some information about Cardiovascular Suite and about the current study. Regarding the study, the study ID is displayed together with information about the patient and the institute. Information about the software, such as version and type of license, are shown in the upper part of the panel.





The home  button closes the FMD Studio application and returns to the home screen of Cardiovascular Suite.


The Archive button  closes the FMD Studio application and returns to the archive of Cardiovascular Suite.

The New video button  allow to open a new video for the analysis.







The Tags Management  button opens the tag management panel as described in [Tags](#).


The preset management  button opens the preset management panel as described in [Presets](#).


The Setup Panel  button is used to show the setup panel when it is hidden.

The Info  button shows information about active controls (calibration lines, ROI, etc.).


The start/pause and save buttons works in a different way for offline analysis and real-time analysis:

- In **offline analysis**, the Start the Analysis  / Pause the Analysis  button starts and suspend the image analysis. The Save the Document  button, saves the document.
- In **real-time analysis**, the Start Recording  / Pause Recording  button starts and suspend both the image recording and the image analysis. The Stop Recording ad Save  button, stops the image recording (i.e. stops the examination) and saves the document.

The Cancel the analysis  button discard the data that have been collected so far.

The Review Documents  button allows to suspend the analysis and to review the documents saved in the current analysis session. The button is only activated if you saved at least one document.

11.2.2 Video window

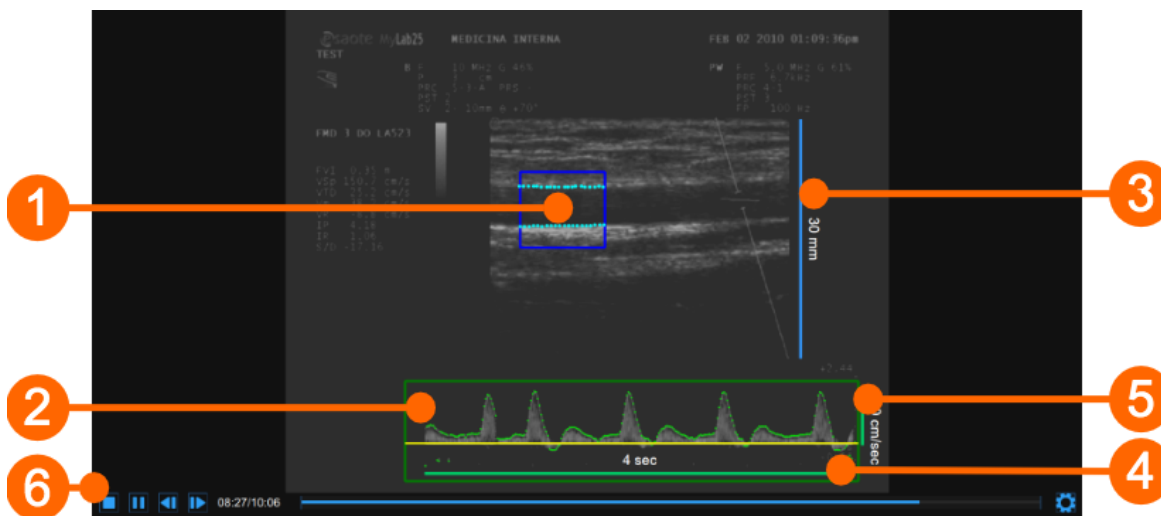


The video window shows the video signal from your ultrasound system. Two ROIs can be present in the window: the diameter ROI in blue **(1)** and the Doppler flow ROI in green **(2)**.

The window contains also the calibration lines for the B-mode image **(3)** and for the Doppler flow **(4)(5)**, once these have been calibrated.

The video controls bar **(6)** is located at the bottom of the window. For more information on the video controls, see [Video and image player](#).

11.2.2.1 Diameter ROI


The Diameter Region of Interest (ROI) is the portion of the image where the diameter is calculated. The edges of the vessel obtained by the algorithm of edge detection are displayed within the ROI. The ROI can be moved and/or resized. Each time you change the position and/or size of the ROI, the contours of the vessel are re-initialized.

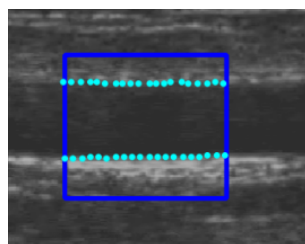


Draw a new diameter ROI:

You can manually draw the diameter ROI with the desired size and position. If the image is already calibrated, you can also more quickly draw a diameter ROI with the default sizes set in [FMD Studio settings](#) (a star in the Set ROI button will indicate that the default ROI can be drawn).

default ROI drawing


- Click on the Set ROI  button in the [Setup panel](#) (the button remains active).
- Click in the video window in the center of the brachial artery.
- A ROI of the default ROI sizes will be automatically initialized.


manual drawing

- Click on the Set B-Mode ROI  button in the [Setup panel](#) (the button remains active).
- Click inside the video window and drag until the Diameter ROI is complete (the size of the ROI is shown in the [Setup panel](#)).
- When you release the mouse, the contours are initialized.

Modify the diameter ROI:



- Click on one of the sides or one of the corners of the diameter ROI.
- Drag to change the size of the the diameter ROI.

 As an alternative, you can modify the size of the diameter ROI by typing the value in the [Setup panel](#).




ROI Edit


Size: 10.63 9.47

Move the diameter ROI:



- Click and hold inside the diameter ROI.
- Drag the diameter ROI to the location of interest.

 As an alternative, you can modify the position of the diameter ROI by typing the value in the [Setup panel](#).



ROI Edit

Position 330 239

Re-initialize the edge detection algorithm:

- Click inside the Diameter ROI.


11.2.2.2 Doppler flow ROI

The Doppler Flow Region of Interest (ROI) is the portion of the image that includes the Doppler Flow waveform.


The algorithm for the Doppler Flow analysis, automatically locates the zero line, which is displayed in yellow, and the waveform, which is displayed in green.

The Doppler Flow ROI can be moved and resized. Each time you change the position and size of the ROI, the algorithm is re-initialized and the zero line is re-localized.

For more information on ultrasound setting for Doppler analysis, please see how to [Calibrate the Doppler flow image](#).

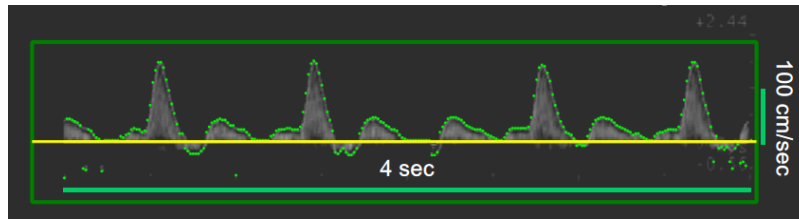



Draw a new Doppler flow ROI:

- Click on the Set Doppler Flow ROI  button in the [Setup panel](#) (the button remains active).
- Click inside the video window and drag until the Doppler Flow ROI is complete (the size of ROI is shown in the [Setup panel](#)).
- When you release the mouse, the algorithm for the Doppler Flow analysis is initialized.

Modify the Doppler flow ROI:


- Click on one of the corners of the Doppler Flow ROI.
- Drag to change the size of the the Doppler Flow ROI (the size of ROI is shown in the [Setup panel](#)).


 As an alternative, you can modify the size of the Doppler flow ROI by typing the value in the [Setup panel](#).



Move the Doppler Flow ROI:

- Click and hold inside the Diameter ROI.
- Drag the Doppler Flow ROI to the location of interest.

 As an alternative, you can modify the position of the Doppler flow ROI by typing the value in the [Setup panel](#).




Re-initialize the algorithm for the Doppler Flow analysis:

- Click inside the Doppler Flow ROI.

Re-initialize the ROI:



- Double click inside the Diameter ROI to re-initialize the position of the ROI

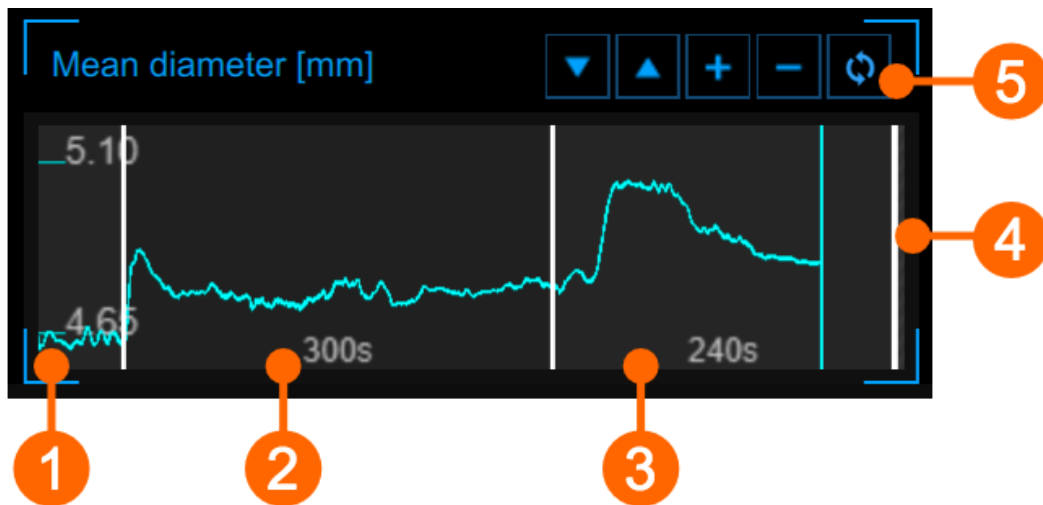11.2.3 Mean diameter chart




The chart shows the trend of the mean diameter during the examination. The chart is divided into three or two parts, according to the study modality. You have basal **(1)**, ischemia **(2)** and vasodilation **(3)** in FMD; ischemia is missing in vasodilation modality. In offline mode, a fourth part **(4)** may be present if the time length of the video is greater than the sum of the basal + (ischemia) + vasodilation.

The time length of the three (two) parts is set in the [Timeline panel](#). You can set the timeline also by moving the three (two) vertical cursors that are present at end-baseline, end-ischemia and end-vasodilation.

Using the buttons at the top right **(5)** you can move up  or down  the chart, enlarge  or reduce  the vertical scale or restore  the default view.

11.2.4 Shear rate chart

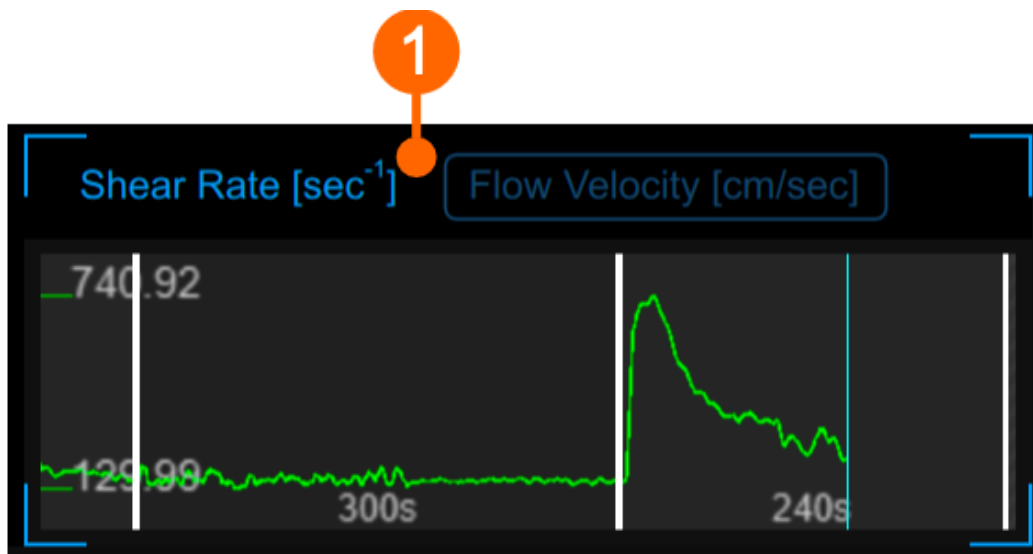


The graph shows the trend of the time averaged positive Shear Rate or the time averaged positive Flow Velocity during the examination. You can switch between the two view by the selector **(1)**.

The chart is divided into time intervals in a similar manner to the [Mean diameter chart](#).



i The chart is enabled if the Doppler analysis has been enabled in the [Setup panel](#).

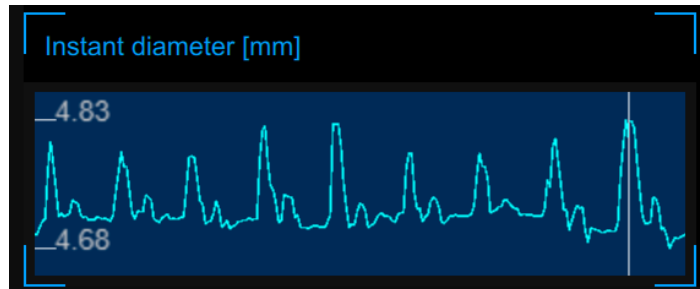11.2.5 Instantaneous diameter chart




This chart shows the diameter changes within the cardiac cycle. The correct form of this chart is an index of measurement quality. The chart axes will automatically scale.

11.2.6 Setup panel

The setup panel contains the commands to set the timeline of the exam, to calibrate the B-mode and the Doppler flow images, to set the diameter and Doppler flow ROIs and to choose the sensitivity of the algorithm. You can move among the panels by using the Next  button and the Previous  button. The Next button is enabled only if you have set all the mandatory field in the panel.

11.2.6.1 Study modality and timeline setup

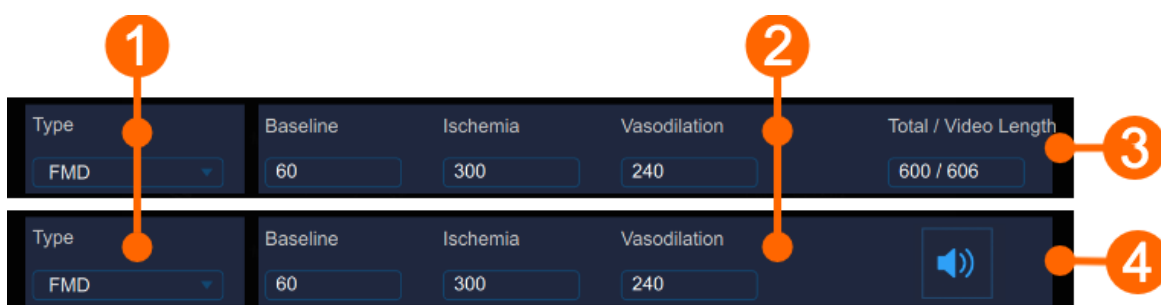

In **(1)**, you can select the study types. FMD Studio can work in two modalities: "FMD" and "Vasodilation". The two modalities differ in how the timeline of the examination is organized.



In **FMD modality**, the timeline is divided into three parts:


1. Baseline, where the software computes the baseline diameter and the baseline shear-rate.
2. Ischemia, which is not used for the analysis.
3. Vasodilation, where the software computes the maximum diameter, the recovery diameter, the maximum shear-rate and the area under the curve of the shear-rate.

In **Vasodilation modality**, the timeline is divided into two parts:

1. Baseline, where the software computes the baseline diameter and the baseline shear-rate.
2. Vasodilation, where the software computes the maximum diameter, the maximum shear-rate and the area under the curve of the shear-rate.

The time length of the timeline parts can be set in the Time panel **(2)**. In the Time Panel, you can choose the time length of baseline, ischemia and vasodilation (ischemia is present only in "FMD" modality) intervals.


In Offline analysis **(3)**, the Time panel shows the total length of baseline + ischemia + vasodilation, and the video length. In Online analysis **(4)**, the panel contains the control indicating if the acoustic alert is Enabled  or Disabled  (click on the icon to change its status). In enabled, an acoustic signal is played at the end of the baseline and the ischemia time interval.

Once the time lengths have been set, click on the Next  button to proceed.

Timeline management

User can set and modify the time length entering values into the Text Fields (see previous picture) but also dragging one of the vertical cursors in graphs, as shown in the following picture:




FMD Studio allows the users to manage the timeline in a flexible way able to meet their clinical and/or research needs. There are constraints on the timeline in terms of minimum and maximum allowed values for each interval (you can not set values outside the allowed range and, if the video modality is "Offline analysis", the sum of the intervals cannot be greater than the time length of the video file under examination). There are also suggested minimum values: if the user decides to ignore this advice, the analysis will be performed anyway but there will be a yellow alert icon () next to the values that may not be reliable in that configuration. In the following table allowed and suggested values are shown:

Timeline constraints (in seconds)			
	Baseline	Ischemia	Vasodilation
FMD	5* - 180	0 - 420	5** - 1200
Vasodilation	5* - 300	-	5 - 1500

* we suggest a basal period of at least 20 sec.

** we suggest a vasodilation period of at least 120 sec.


If the user uploads a video clip (for offline analysis) with a lower duration than the minimum allowed values (it means 10 seconds; 5 for baseline and 5 for vasodilation) an error message will appear: "This video is less than 10 sec long. You will be able to analyse the video but only instantaneous values will be generated. FMD value will not be calculated."

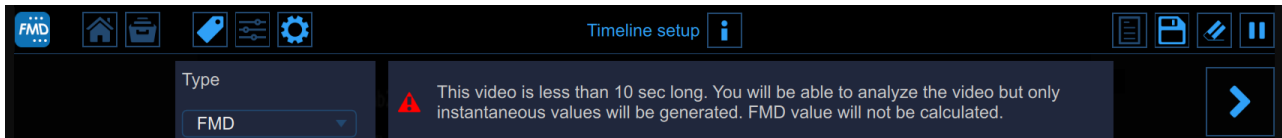

In this configuration user cannot set the timeline and characteristics parameters (e.g. FMD, FMDr, baseline diameter,...) will not be computed but only instantaneous values will be generated.


You can hover over the yellow icon (⚠️) or the red one (🚨) and an informative message about the warning or error situation will be displayed.

11.2.6.2 B-mode image setup

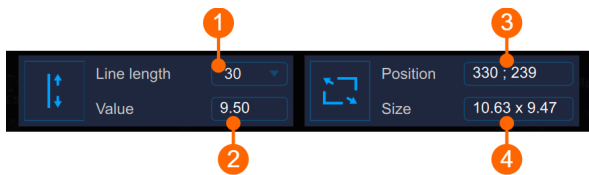


The B-Mode Panel must be used to [Calibrate the B-mode image](#) and to set the diameter ROI.


Calibration

The Set B-Mode Calibration  button is used to [Calibrate the B-mode image](#).


The drop down menu **(1)** shows the length of the line used for the calibration.

The numeric display **(2)** shows the calibration value.

 If you click in the value field, you are allowed to manually enter the calibration value in the editable field (if you already know the value). Then click the Save button to save the values.



ROI

The Set B-Mode ROI  button is used to set the diameter ROI.

The numeric display **(3)** shows the center position, in pixels, of the diameter ROI.

The numeric display **(4)** shows the size (width x height), in mm, of the diameter ROI.


i If you click in the value field, you are allowed to manually enter the ROI position and size values in the editable fields (if you already know the values). The click the Save button to enter the values.

ROI Edit


Position

ROI Edit

Size:

Once you have calibrated the B-Mode image and set the Diameter ROI, click on the Next  button to proceed.

11.2.6.3 Doppler Setup

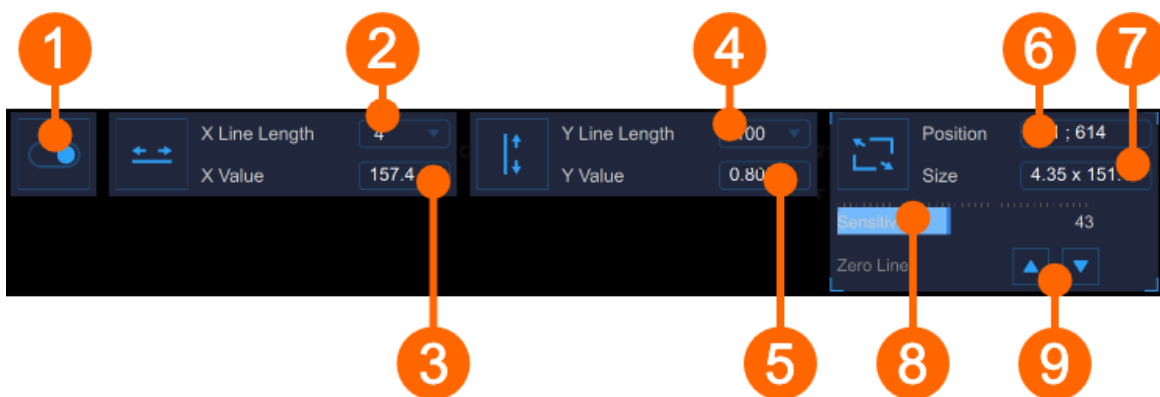

The Doppler Panel must be used to [Calibrate the Doppler flow image](#) and to set the Doppler flow ROI.

The switch **(1)** enables and disables the Doppler Flow analysis.

Calibration

The Set Doppler X-Calibration  button is used to calibrate the x-axis (time).

The drop down menu **(2)** shows the length of the line used for the calibration (sec).

The numeric display **(3)** shows the x-calibration value (pix/sec).

The Set Doppler Y-Calibration  button is used to calibrate the y-axis (velocity).

The drop down menu **(4)** shows the length of the line used for the calibration (cm/sec).

The numeric display **(5)** shows the y-calibration value (pix/cm/sec).

ROI

The Set Doppler Flow ROI  button is used to set the Doppler flow ROI.

The numeric display **(6)** shows the center position, in pixels, of the Doppler flow ROI.


The numeric display **(7)** shows the size (width x height), in pixels, of the Doppler flow ROI.


The sensitivity of the Doppler Flow analysis algorithm is set by the slider **(8)**.

The position of the zero line can be adjusted by the buttons **(9)**.

Once you have calibrated the B-Mode image and set the Diameter ROI, click on the Next  button to proceed.


11.2.7 Tags

The Tags Management  button opens a panel that allows to associate a tag to the document, or create a new tag. Tags can also be managed through the Tags management into the Archive.

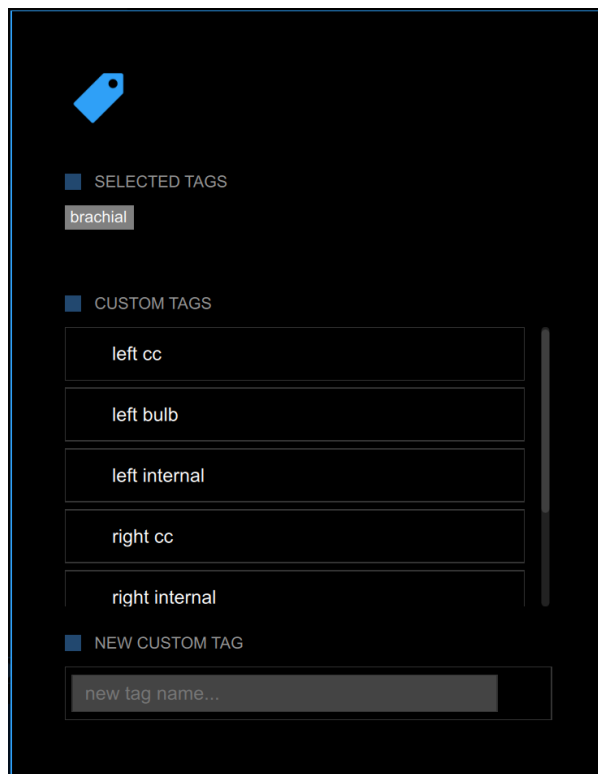


The selected tags are visible in a special area of the Analysis window. The tags area can be moved by right clicking and dragging.

11.2.8 Presets

The preset management button  opens the preset management panel that allows to manage presets. In particular, it allows to remember the settings of:

- timeline (baseline, ischemia and vasodilation)
- B-mode image calibration
- B-mode image ROI (size and position)
- Doppler calibration (X and Y calibration)
- Doppler ROI (size and position)


A preset can be saved and reused for following studies.

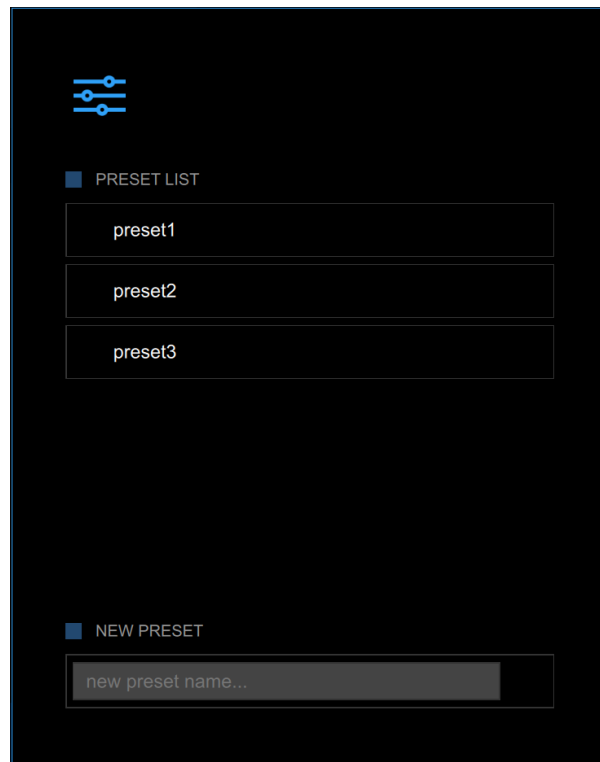


11.2.9 Calibrate the B-mode image


The calibration of the images must be done before starting a new examination because it is necessary to provide information about the size of the image generated by ultrasound system. The calibration factor changes depending on the settings of your ultrasound machine. You should check the calibration at each new examination.


⚠ CAUTION: the lack of calibration can generate a software malfunction.

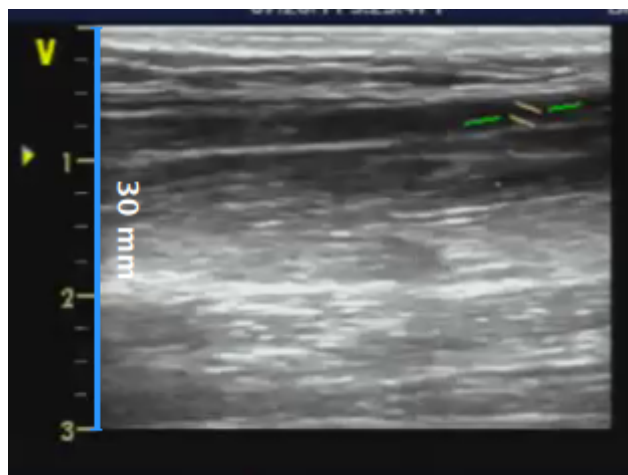

- Locate, in ultrasound image, a range of known distance (30 mm. in the example of figure).
- In the B-mode setup panel, select from the drop-down menu, the distance specified above.

- In the B-mode setup panel, click on the Set B-Mode Calibration  button (button remains active).
- Draw a line on the image corresponding to the known distance: click on one end and drag the mouse to the other extreme (press the Shift key or Ctrl+Shift keys on your keyboard if you want the line to be not vertical or horizontal).


 For DICOM files, when present, the B-mode calibration is obtained automatically by the file metadata (see [Settings](#)). You can anyhow modify the calibration value.



 You can directly type the calibration value in the Calibration factor field of the B-mode setup panel, if you already know the value.

11.2.10 Calibrate the Doppler flow image

The calibration of the Doppler Flow analysis must be done before starting a new examination because it is necessary to provide information about the size of the Doppler waveform generated by ultrasound system. The calibration factor changes depending on the settings of your ultrasound machine. You should check the calibration at each new examination.

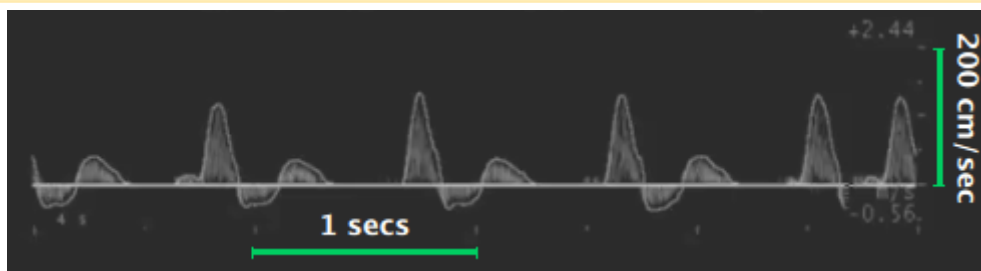 **CAUTION: the lack of calibration can generate a software malfunction.**




- Locate, on the x axis of the Doppler flow profile, a known time length (1 sec in the example in figure).
- In the Doppler setup panel, select from the "x-line length" drop-down menu, the time length specified above.
- In the Doppler setup panel, click on the Set Doppler X-Calibration  button (button remains active).
- Draw a line on the image corresponding to the known distance: click on one end and drag the mouse to the other extreme (press the Shift key on your keyboard if you want the line to be not horizontal).
- Locate, on the y axis of the Doppler flow profile, a known flow velocity value (200 cm/sec in the example in figure).
- In the Doppler setup panel, select from the "y-line length" drop-down menu, the flow velocity value specified above.
- In the Doppler setup panel, click on the Set Doppler Y-Calibration  button (button remains active).
- Draw a line on the image corresponding to the known distance: click on one end and drag the mouse to the other extreme (press the Shift key on your keyboard if you want the line to be not vertical).

i For DICOM files, when present, the Doppler calibration is obtained automatically by the file metadata (see [Settings](#)). You can anyhow modify the calibration values.


✓ You can directly type the calibration values in the X value and Y value fields of the Doppler setup panel (if you already know the values).

11.2.11 Doppler flow analysis

FMD Studio computes the envelope of the Doppler flow velocity waveform over the time interval defined by the Doppler flow ROI. The result is used to compute the Time Average Wall Shear Rate.

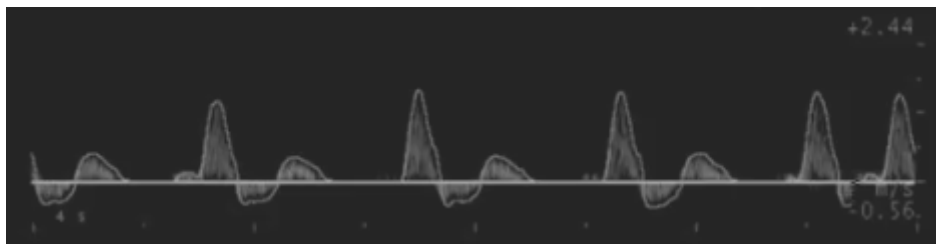

We assume the velocity profile to be parabolic and we assume that the Doppler flow velocity waveform provides the maximum value (VM) of the velocity profile (i.e. the maximum spatial velocity). In fact, the analysis is based only on the Doppler flow envelope because the video image data does not give information on the velocity profile of the vessel.

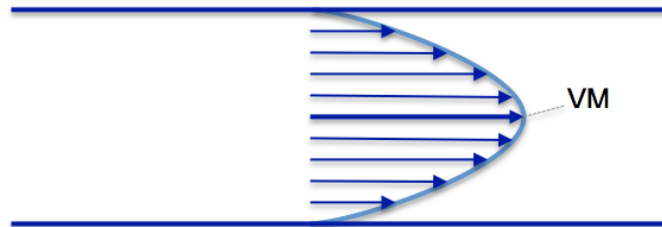

Velocity Profile in a vessel

With this assumptions, the Shear Rate (SR) can be computed as:

$$SR = \frac{4 \cdot V}{d}$$


where d is the diameter of the vessel.

FMD Studio computes two values for velocity:

V_{TAP} : time averaged of the positive values of V.

V_{TAN} : time averaged of the negative values of V.

Both the averages are computed over the Doppler flow ROI.

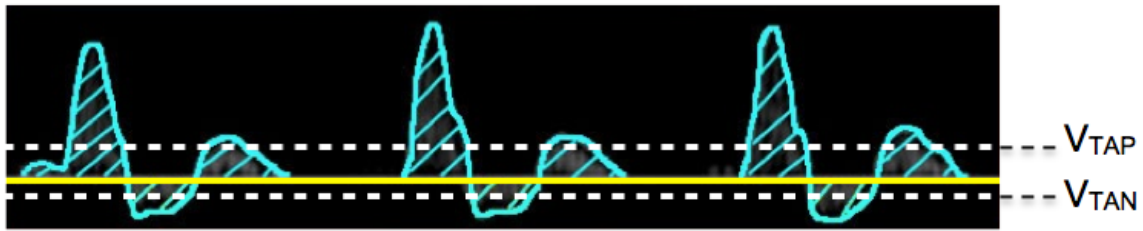


These two values are used to compute the Shear Rate as:

SR_{TAP} : Time Average Positive wall Shear Rate.

SR_{TAN} : Time Average Negative wall Shear Rate.

11.3 Review

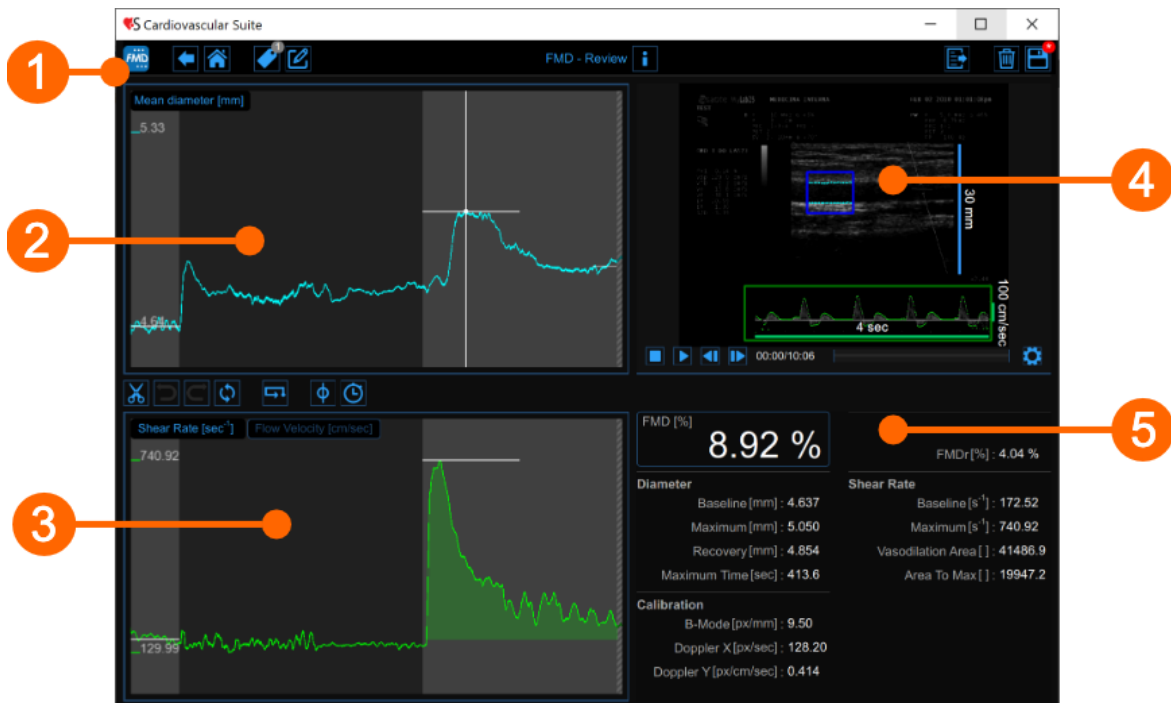

The Review window shows the result of the analysis and allows you to remove piece of data that are considered to be "outliers". This can happen, for example, if in a short time interval the patient did move and the brachial artery was not correctly displayed. In the Review window you can review both the images and the result of the analysis and decide to remove the data that were generated in this time interval.


The Review window contains the following components:


1. Top bar
2. Mean diameter chart
3. Shear rate chart
4. Video window
5. Results panel


11.3.1 Top bar


The top bar contains some essential information for the navigation.




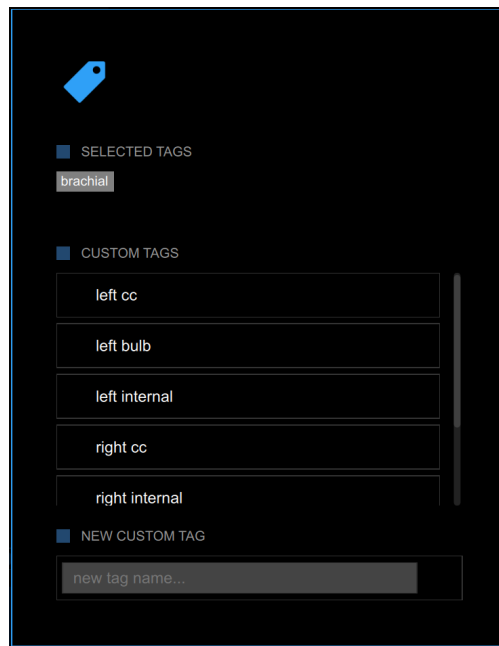
The FMD Studio  button shows a panel containing some information about Cardiovascular Suite, about the current study and the current document. Regarding the study, the study ID is displayed together with information about the patient and the institute. In addition, info regarding the current document are provided. Information about the software, such as version and type of license, are shown in the upper part of the panel.

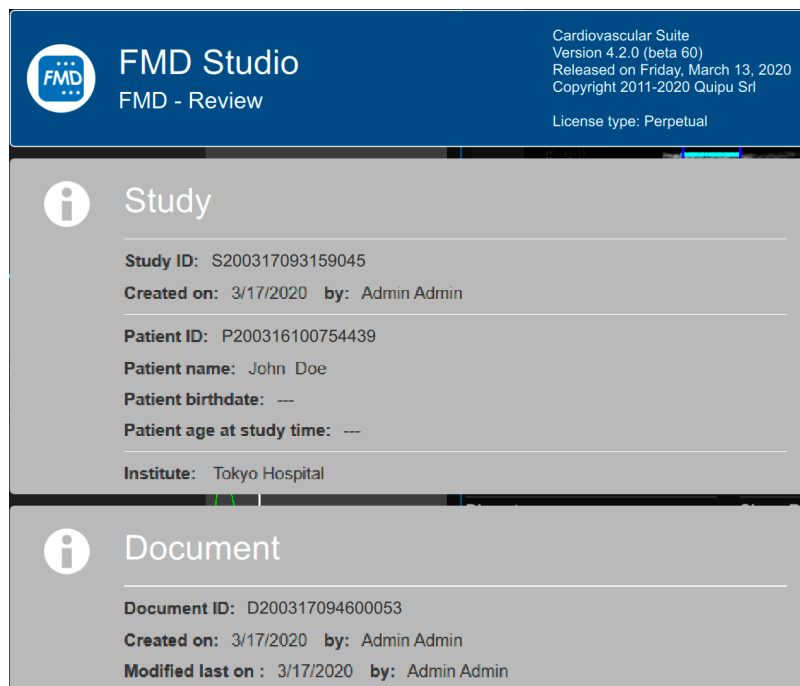


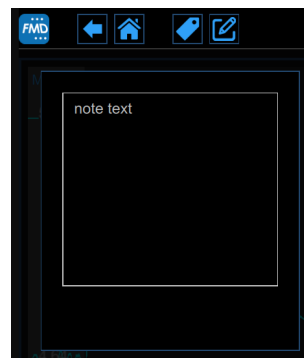
The Home  button closes the FMD Studio application and returns to the home screen of Cardiovascular Suite.


The back  button closes the FMD Studio application and comes back to the Archive.


The Tags Management  button opens a panel (see the following picture) that allows to create a new tag and associate it or an existing tag to the document. Tags can be managed through the [Tags management](#) into the Archive.




The Notes  button can be used to enter a note in the document.




The Save  button is used to save your changes to the document once you have edited the data.

The Delete the document  button is used to delete the current document.


The Export  button is used to export your data. You can export the Document Results and the Document Data.

The **Document Results** contains all the results of the analysis and all the information about the study, the document, and the patient.

The **Document Data** contains all the Document Results, a list of the Mean Diameter, the Shear Rate, and the Doppler Velocity (one value per second) and the Diameter and the Doppler Velocity values computed at each frame.

 Only the diameter values are actual instantaneous values because they are computed on the single images. The Doppler Velocity is actually a Time averaged value. In fact, despite it is calculated on the single image, it is computed in the time interval defined by the Doppler flow ROI. For more info, please see [Doppler flow analysis](#).



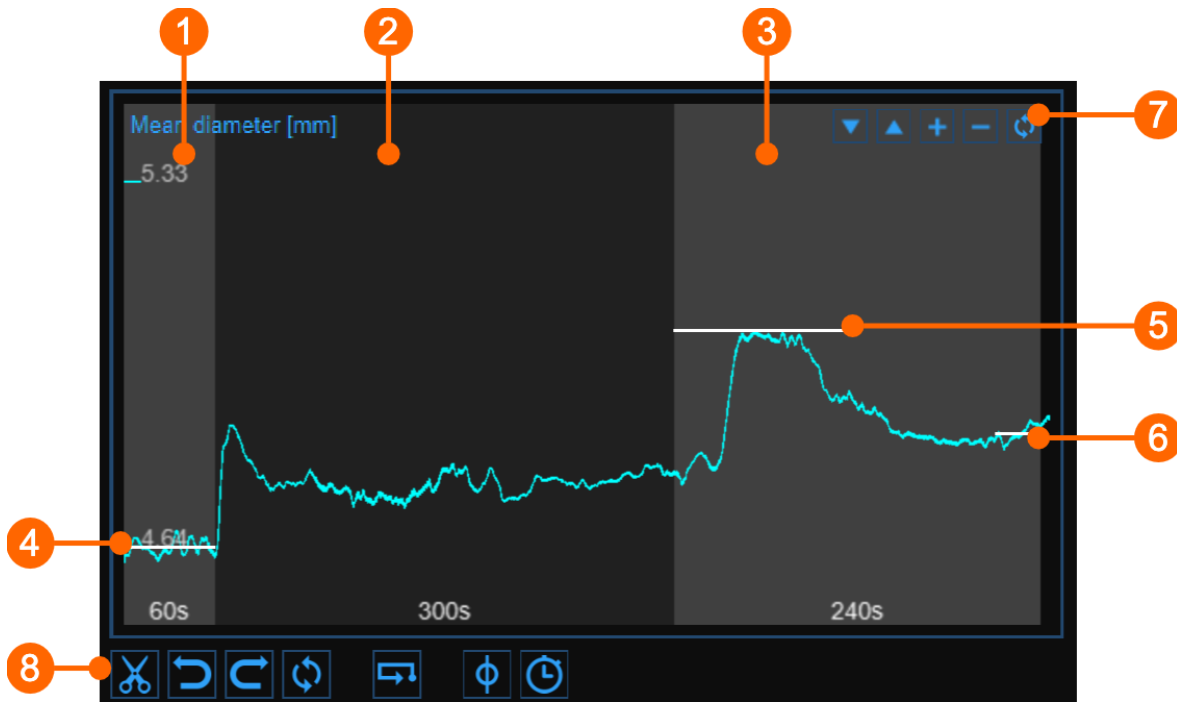


11.3.2 Mean diameter chart



The chart shows the trend of the mean diameter during the examination. The chart is divided into three or two parts, according to the study modality. You have basal **(1)**, ischemia **(2)** and vasodilation **(3)** intervals in FMD; ischemia is missing in vasodilation modality.



In the chart, three cursors are present (two cursors in "Vasodilation" study mode): the first one **(4)** is placed at the baseline diameter value; the second one **(5)** is placed at the maximum diameter value in vasodilation; the third one **(6)** is placed at the post baseline (this cursors is absent in "Vasodilation" study modality). Cardiovascular Suite places the cursors at the position automatically computed at the end of the analysis. You can manually place these values if you see that some outliers have affected the automatic analysis.




These values are shown in the [Results panel](#).


Using the buttons at the top right **(7)** you can move up  or down  the chart, enlarge  or reduce  the vertical scale or restore  the default view.

The buttons under the chart **(8)** can be used for editing the chart in order to remove the outliers, for activating the graph cursor, and for modifying the timeline.


11.3.2.1 Remove the outliers


- Click on the Cut  button.
- In the Mean diameter chart, click on one of the two extremes of the range to be deleted.
- Drag the mouse horizontally to the other extreme of the range to be deleted (see next paragraph for removal constraints).
- Once you have removed the outliers, click on the recompute  button if you want to re-analyze the data on the edited chart.

You can use the undo  and redo  buttons to cancel and restore your changes. The restore  button cancels all your changes and restore original data.


✓ Click on the Save  button in the [Top bar](#) to save your changes to the document.

11.3.2.2 Graph cursors

As shown in the following figure, the Cursor  button **(1)** activates a cursor **(2)** on the Mean Diameter chart that shows the current time position on the graph according to the images shown in the [Video window](#). The coordinates (diameter value in millimeters and time value in the format *minutes:seconds.milliseconds*) of the cursor are dynamically updated and shown in **(3)**. When the Cursor button is active, it is also possible to know the coordinates of an exact point in the graph; it is only needed to hover over the chart and a second cursor **(4)** is displayed. It follows the mouse movements and the exact coordinates of the point are shown in the label **(5)** (diameter value is expressed in millimeters and the time value has the format *minutes:seconds.milliseconds*).

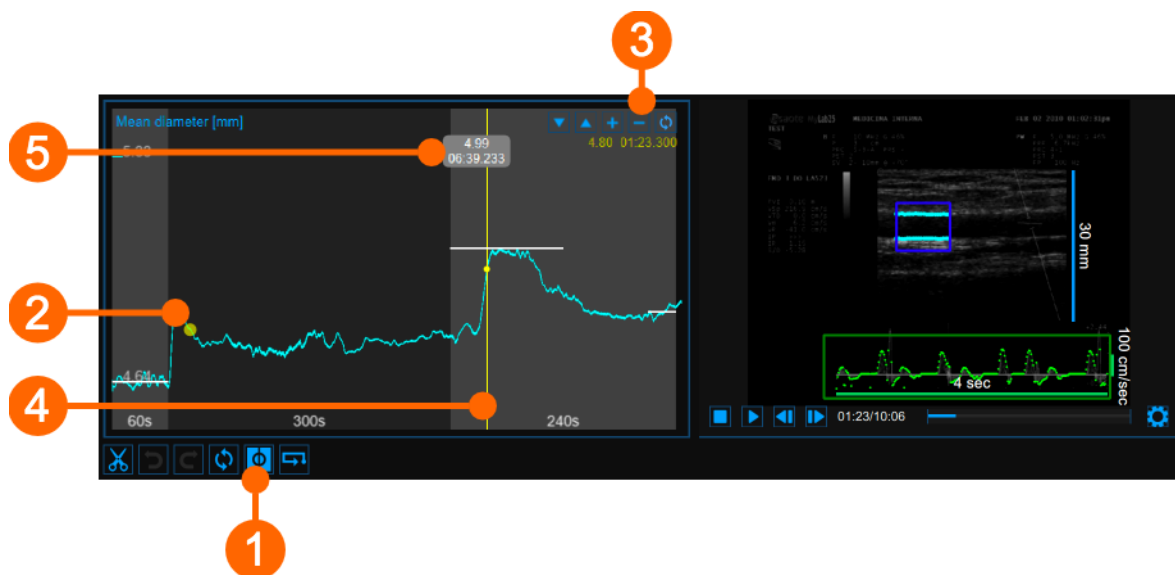

11.3.2.3 Modify the timeline

- Click the Timeline  button **(4)**.
- Move the vertical cursors that are placed at the end-baseline **(1)**, end-ischemia **(2)** and end-vasodilation **(3)**.




11.3.2.4 Alerts

In FMD Studio Review you can cut and delete data from the mean diameter chart. Please, note that timeline constraints are already valid (see **Timeline management** paragraph in [Setup panel](#)).

After data removal, if there are intervals with a duration lower than the suggested value or than the allowed value, a yellow (⚠️) or red (🚫), respectively, alert icon will appear next to the parameters that can be affected by the too short time interval. In addition, if the intervals do not meet the minimum duration allowed value some parameters will not be calculated. You can hover over the icons and an informative message about the warning or error situation will be displayed.

11.3.3 Shear rate chart

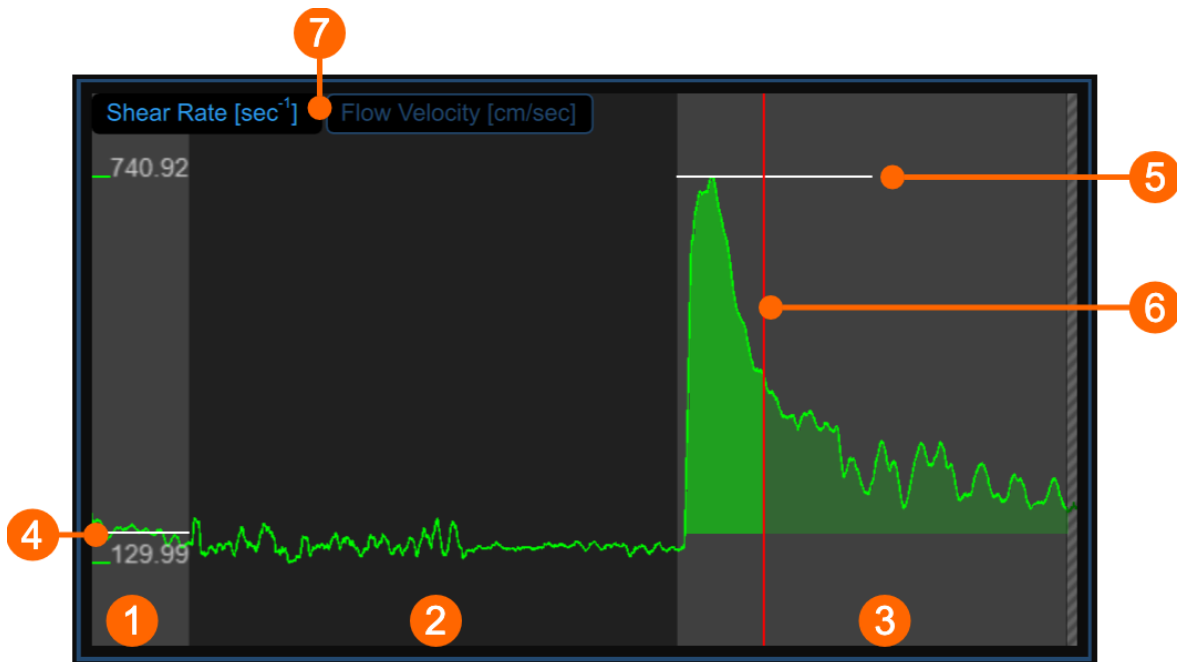


The chart shows the trend of the time averaged positive Shear Rate (or the time averaged positive Flow Velocity, according to selector **(7)**) during the examination. The chart is divided into three or two parts, according to the study modality. You have basal **(1)**, ischemia **(2)** and vasodilation **(3)** intervals in FMD; ischemia is missing in vasodilation modality.

In the chart, two cursors are present: the first one **(4)** is placed at the baseline value; the second one **(5)** is placed at the maximum value in vasodilation. A third cursors **(6)** is shown at the time value corresponding to the maximum value of the diameter when the same cursor is selected in the [Mean diameter chart](#). Cardiovascular Suite places the cursors at the position automatically computed at the end of the analysis. You can manually place these values if you see that some outliers have affected the automatic analysis.


These values are shown in the [Results panel](#).

11.3.3.1 Graph cursors

As shown in the following figure, the Cursor  button at the bottom of the [Mean diameter chart](#) activates a cursor **(1)** on the Shear rate chart that shows the current time position on the graph according to the images shown in the [Video window](#). The coordinates (shear rate value in s^{-1} and time value in the format *minutes:seconds.milliseconds*) of the cursor are dynamically updated and shown in **(2)**. When the Cursor button is active, it is also possible to know the coordinates of an exact point in the graph; it is only needed to hover over the chart and a second cursor **(3)** is displayed. It follows the mouse movements and the exact coordinates of the point are shown in the label **(4)** (shear rate value is expressed in s^{-1} and the time value has the format *minutes:seconds.milliseconds*).




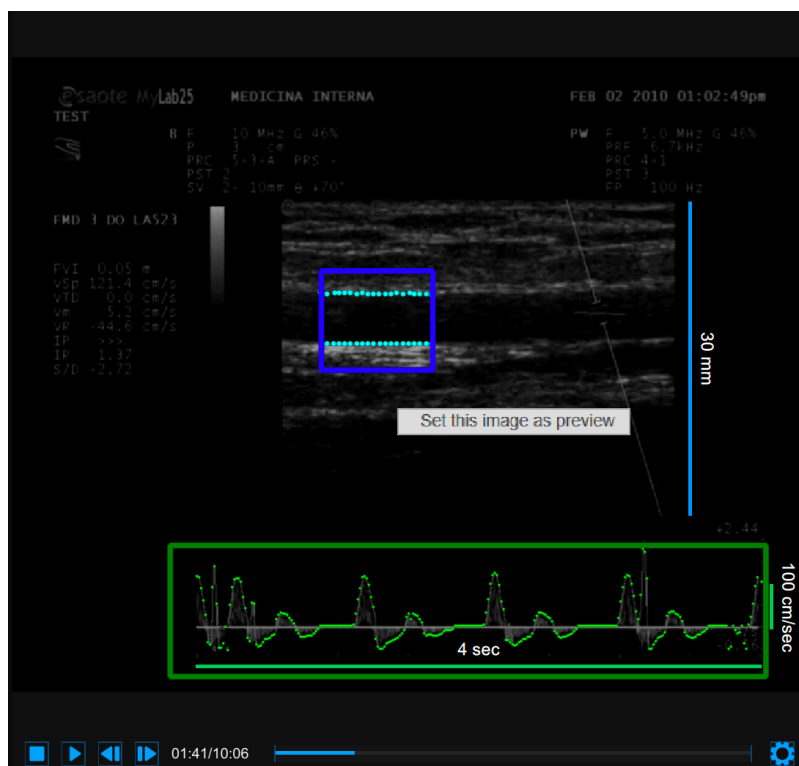
11.3.4 Video window

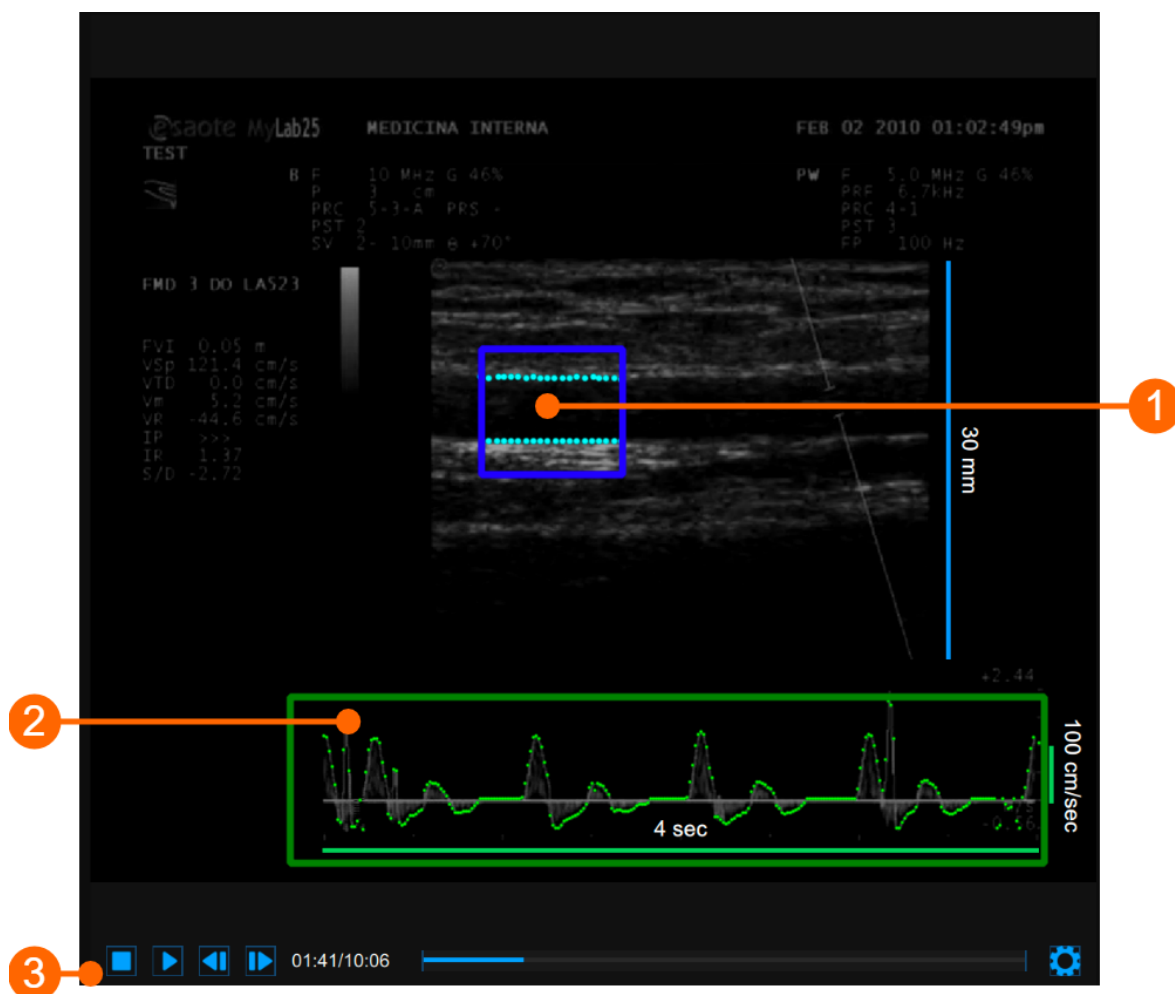

The video window shows the video signal from your ultrasound system. Two ROIs can be present in the window: the diameter ROI in blue **(1)** and the Doppler flow ROI in green **(2)**.


The Video control bar **(3)** is located at the bottom of the window.

If you want to expand the video window, you have to click on the Enlarge  button.



i If you perform right click on the video window and click on "Set this image as preview" the current frame will be saved and displayed in the Documents Table as document preview (see [Studies management](#))

11.3.5 Results panel

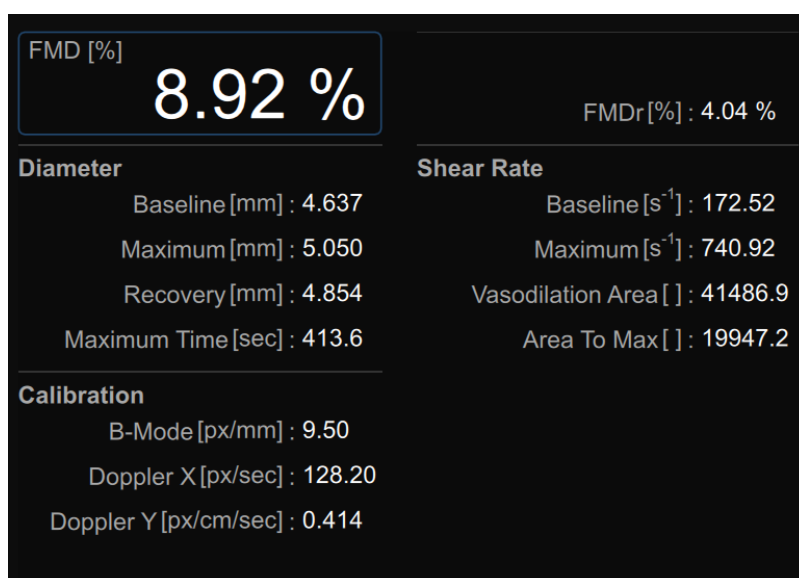

The panel shows the results of the analysis. The following data are displayed:

- **FMD [%]: Flow Mediated Dilation**

$$FMD = \frac{\text{Maximum Diameter} - \text{Baseline Diameter}}{\text{Baseline Diameter}}$$

- **FMD_r [%]: Flow Mediated Dilation with respect to the Recovery Diameter**

$$FMD_r = \frac{\text{Maximum Diameter} - \text{Recovery Diameter}}{\text{Recovery Diameter}}$$

Diameter

- **Baseline Diameter [mm]:** mean of the diameter values in the "Baseline" time interval.
- **Maximum Diameter [mm]:** maximum diameter value in the "Vasodilation" time interval.
- **Recovery Diameter [mm]:** mean of the last 30 seconds of diameter values available in the "Vasodilation" time interval.
- **Maximum Time [sec]:** time of the maximum diameter value in the "Vasodilation" time interval.

Calibration

- **B-Mode calibration value [px/mm]:** value of the calibration of the B-mode image
- **Doppler X calibration value [px/sec]:** value of calibration of the x axis (time) of PW Doppler
- **Doppler Y calibration value [px/cm/sec]:** value of calibration of the y axis (velocity) of PW Doppler

Shear Rate *(visible when the shear rate chart is visible)*

- **Baseline Shear Rate [s⁻¹]:** mean of the shear rate values in the Baseline time interval.
- **Maximum Shear Rate [s⁻¹]:** maximum of the shear rate values in the Vasodilation time interval.
- **Vasodilation Area [dimensionless]:** area under the curve of the shear rate in the Vasodilation time interval, calculated with reference to the baseline shear rate value (Fig. 1).
- **Area to Max [dimensionless]:** area under the curve of the shear rate in the time interval that begins with the Vasodilation and ends at the time of the Maximum Diameter, calculated with reference to the baseline shear rate value (Fig. 2).

Flow Velocity *(visible when the flow velocity chart is visible)*

- **Baseline Flow Velocity [cm/sec]:** mean of the flow velocity values in the Baseline time interval.
- **Maximum Flow Velocity [cm/sec]:** maximum of the flow velocity values in the Vasodilation time interval.
- **Vasodilation Area [cm]:** area under the curve of the flow velocity in the Vasodilation time interval, calculated with reference to the baseline flow velocity value (Fig. 1).
- **Area to Max [cm]:** area under the curve of the flow velocity in the time interval that begins with the Vasodilation and ends at the time of the Maximum Diameter, calculated with reference to the baseline flow velocity value (Fig. 2).

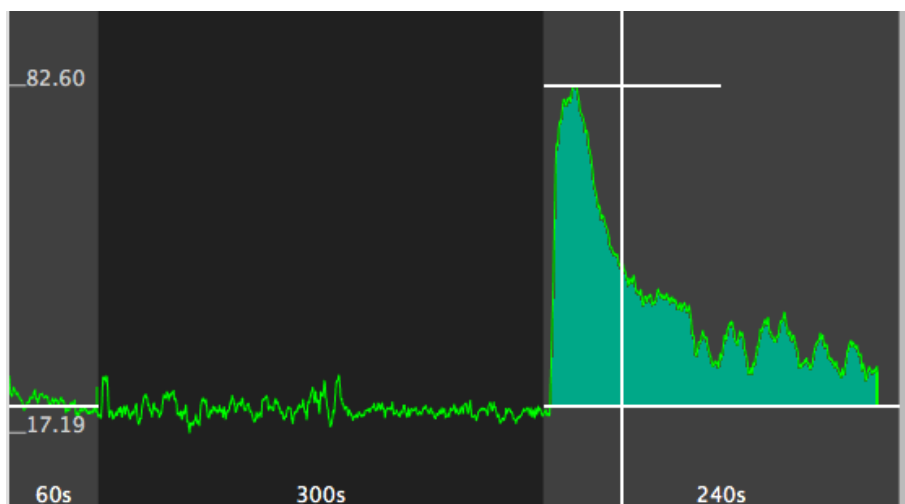


Figure 1 - Area

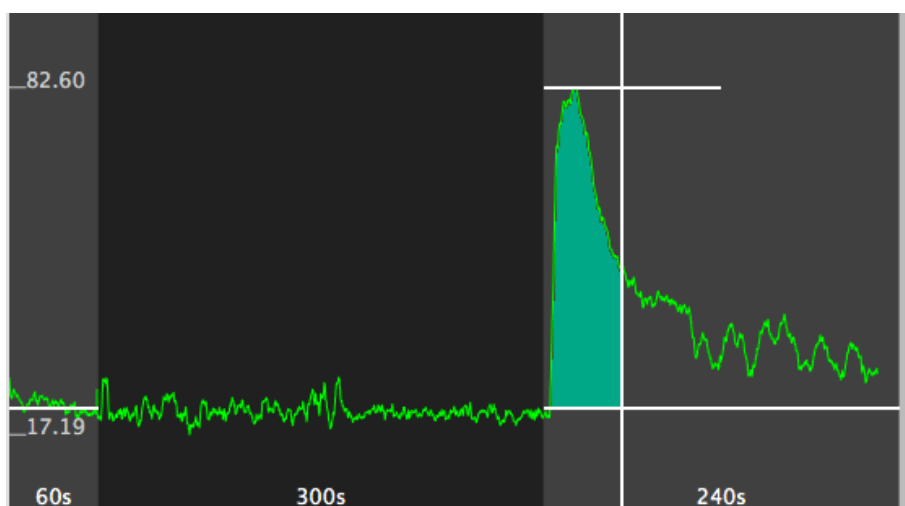


Figure 2 - Area to Max

These data can also be exported in different formats. See [here](#) for export details.

12 Warnings



This software may provide incorrect results in the following cases:

- if recommendations regarding type of analysed images, adopted ultrasound equipment and experience of the operator are not followed;
- if the user does not perform the basic operations required, such as calibration and proper tracking of initial contours.

Essential requirement for a correct analysis is the operation of the device. In case of a fault:

- close and reopen the application software, or
- restart the computer where the software is installed and open the application again
- contact your dealer for assistance.

Any malfunction of the device, however, does not affect the state of health of the patient.

The user has the responsibility to check the accuracy of the external ultrasound images to avoid the possibility of generating an incorrect result.

The software device must be used in an environment that allows optimal visibility of the screen.

The software device has a 2 years warranty in which Quipu will provide security updates.

13 References

- Gemignani V, Faita F, Ghiadoni L, Poggianti E, Demi M.
“A system for real-time measurement of the brachial artery diameter in B-mode ultrasound images.”
IEEE Trans Med Imaging. 2007 Mar;26(3):393-404.
- Gemignani V, Bianchini E, Faita F, Giannarelli C, Plantinga Y, Ghiadoni L, Demi M.
“Ultrasound measurement of the brachial artery flow-mediated dilation without ECG gating”
Ultrasound Med Biol. 2008 Mar;34(3):385-91. Epub 2007 Oct 26.
- Faita F, Gemignani V, Bianchini E, Giannarelli C, Ghiadoni L, Demi M.
“Real-time measurement system for evaluation of the carotid intima-media thickness with a robust edge operator.”
J Ultrasound Med. 2008 Sep;27(9):1353-61
- Bianchini E, Bozec E, Gemignani V, Faita F, Giannarelli C, Ghiadoni L, Demi M, Boutouyrie P, Laurent S.
“Assessment of carotid stiffness and intima-media thickness from ultrasound data: comparison between two methods.”
J Ultrasound Med. 2010 Aug;29(8):1169-75.
- E. Bianchini, A. Corciu, L. Venneri, F. Faita, C. Giannarelli, V. Gemignani, M. Demi.
"Assessment of Cardiovascular Risk Markers from Ultrasound Images: System Reproducibility."
Computers in Cardiology 2008;35:105–108.
- Faita F, Masi S, Loukogeorgakis S, Gemignani V, Okorie M, Bianchini E, Charakida M, Demi M, Ghiadoni L, Deanfield JE.
“Comparison of two automatic methods for the assessment of brachial artery flow-mediated dilation.”
J Hypertens. 2011 Jan;29(1):85-90.
- Ghiadoni L, Faita F, Salvetti M, Cordiano C, Biggi A, Puato M, Di Monaco A, De Siati L, Volpe M, Ambrosio G, Gemignani V, Muiesan M, Taddei S, Lanza GA, Cosentino F.
“Assessment of Flow-Mediated Dilation Reproducibility: a Nationwide Multicenter Study”.
J Hypertens. 2012 Jul;30(7):1399-405
- Charakida M, Masi S, Lüscher TF, Kastelein JJ, Deanfield JE.
“Assessment of atherosclerosis: the role of flow-mediated dilatation.”
Eur Heart J. 2010 Dec;31(23):2854-61. Epub 2010 Sep 23.

- Yeboah J, Crouse JR, Hsu FC, Burke GL, Herrington DM.

“Brachial flow-mediated dilation predicts incident cardiovascular events in older adults: the Cardiovascular Health Study.”

Circulation. 2007 May 8;115(18):2390-7. Epub 2007 Apr 23.

- O'Leary DH, Bots ML.

“Imaging of atherosclerosis: carotid intima-media thickness.”

Eur Heart J. 2010 Jul;31(14):1682-9. Epub 2010 Jun 11.

- Amato M, Veglia F, de Faire U, Giral P, Rauramaa R, Smit AJ, Kurl S, Ravani A, Frigerio B, Sansaro D, Bonomi A, Tedesco CC, Castelnovo S, Mannarino E, Humphries SE, Hamsten A, Tremoli E, Baldassarre D; IMPROVE study group.

"Carotid plaque-thickness and common carotid IMT show additive value in cardiovascular risk prediction and reclassification."

Atherosclerosis. 2017 Aug;263:412-419.

- Mattace-Raso FU, van der Cammen TJ, Hofman A, van Popele NM, Bos ML, Schalekamp MA, Asmar R, Reneman RS, Hoeks AP, Breteler MM, Witteman JC.

“Arterial stiffness and risk of coronary heart disease and stroke: the Rotterdam Study.”

Circulation. 2006 Feb 7;113(5):657-63.

- Lian Engelen, Isabel Ferreira, Coen D Stehouwer, Pierre Boutouyrie, Stéphane Laurent, Reference Values for Arterial Measurements Collaboration

"Reference intervals for common carotid intima-media thickness measured with echotracking: relation with risk factors"

Eur Heart J. 2013 Aug;34(30):2368-80. Epub 2012 Nov 27.

- Lian Engelen, Jelle Bossuyt, Isabel Ferreira, Luc M van Bortel, Koen D Reesink, Patrick Segers, Coen D Stehouwer, Stéphane Laurent, Pierre Boutouyrie, Reference Values for Arterial Measurements Collaboration

"Reference values for local arterial stiffness. Part A: carotid artery"

J Hypertens. 2015 Oct;33(10):1981-96.



14 Contacts

Quipu S.r.l.

Address:

via Moruzzi 1

I-56124 Pisa Italy

Telephone:

(+39) 050 315 2612

Web:

www.quipu.eu

info@quipu.eu



15 Notes

15.1 Trademarks

Cardiovascular Suite, FMD Studio and Carotid Studio are trademarks of Quipu srl.

Mac, OS X and macOS are registered trademarks of Apple Inc.

Microsoft and Windows are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.

AV.io HD is a trademark of Epiphan Systems Inc.

Magewell is a trademark of Nanjing Magewell Electronics Co.

HDMI is a trademark of HDMI Licensing LLC.

Adobe Acrobat is a trademark of Adobe Inc.

15.2 EULA

End user license agreement for Cardiovascular Suite

Document number: LEG0001EN rev. 8 of July 1st, 2020

Please read this EULA carefully, as it sets out the basis upon which we license the Software for use.

By clicking "accept agreement" when you first install the Software, you agree to be bound by the provisions of this EULA. If you do not agree to be bound by the provisions of this EULA, you must stop the installation now.

By agreeing to be bound by this EULA, you further agree that any person you authorize to use the Software will comply with the provision of this EULA.

By agreeing to be bound by this EULA, you hereby acknowledge that you are familiar with and agree to the terms of the Licensor's privacy policy available at <http://www.quipu.eu/privacy-policy/>

1. Definitions

1.1 Except to the extent expressly provided otherwise, in this EULA:

"Commercial License" means a license to use Software obtained or renewed by the User by paying fees.

"Documentation" means the documentation for the Software produced by the Licensor and delivered or made available by the Licensor to the User.

"EULA" means this end user license agreement, including any amendments to this end user license agreement from time to time.

"Effective Date" means the date upon which the User gives the User's express consent to this EULA, following the issue of this EULA by the Licensor.

"Expiry Date" means such date as may be the ending of the usage of the Software.

"Evaluation License" means a 14 days license according to this EULA, limited only for evaluation of the Software purposes, in accordance with Clause 5.

"Force Majeure Event" means an event, or a series of related events, that is outside the reasonable control of the party affected (including failures of the internet or any public telecommunications network, hacker attacks, denial of service attacks, virus or other malicious Software attacks or infections, power failures,



industrial disputes affecting any third party, changes to the law, disasters, explosions, fires, floods, riots, terrorist attacks and wars).

"Intellectual Property Rights" means all intellectual property rights wherever in the world, whether registrable or unregistrable, registered or unregistered, including any application or right of application for such rights (and these "intellectual property rights" include copyright and related rights, database rights, confidential information, trade secrets, know-how, business names, trade names, trademarks, service marks, passing off rights, unfair competition rights, patents, petty patents, utility models, semi-conductor topography rights and rights in designs);

"Licensor" means Quipu s.r.l., a company incorporated in Italy (registration number 01995110507) having its registered office at via Moruzzi 1 I-56124 Pisa – Italy.

"License Key" means a piece of hardware (USB dongle) provided by the Licensor, which must be plugged into a USB port of the computer where the Software is installed and allows the Software to run.

"Perpetual License" means a license with no specified term or expiration.

"Software" means the Software Cardiovascular Suite.

"Software Defect" means a defect, error or bug in the Software having an adverse effect on the appearance, operation, functionality, or performance of the Software, but excluding any defect, error or bug caused by or arising as a result of:

- any act or omission of the User.
- any use of the Software contrary to the Documentation by the User or any person authorized by the User to use the Software.
- a failure of the User to perform or observe any of its obligations in this EULA; and/or
- an incompatibility between the Software and any other system, network, application, program, hardware, or Software not specified as compatible in the Software Specification.

"Software Specification" means the specification for the Software set out in the Documentation.

"Source Code" means the Software code in human-readable form or any part of the Software code in human-readable form, including code compiled to create the Software or decompiled from the Software, but excluding interpreted code comprised in the Software.

"Term" means the term of this EULA, commencing in accordance with Clause 2.1 and ending in accordance with Clause 2.2.

"Time License" means a time limited license that is granted until the expiry date.

"Update" means a hotfix, patch, or minor version update to the Software;

"Upgrade" means a major version upgrade of the Software.

"User" means the person to whom the Licensor grants a right to use the Software under this EULA.

2. Term

2.1 This EULA shall come into force upon the Effective Date.

2.2 This EULA shall continue in force:

- indefinitely, for Perpetual Licenses; or
- until the expiry date, for Time Licenses; or
- 14 days, for Evaluation Licenses.

subject to termination in accordance with Clause 12.

3. License



3.1 The Licensor hereby grants to the User from the date of supply of the Software to the User until the end of the Term a worldwide, non-exclusive license to:

- install a single instance of the Software.
- use a single instance of the Software in accordance with the Documentation; and
- create, store, and maintain up to 5 back-up copies of the Software,

subject to the limitations and prohibitions set out and referred to in this Clause 3.

3.2 The User may not sub-license and must not purport to sub-license any rights granted under Clause 3.1 without the prior written consent of the Licensor.

3.3 Save to the extent expressly permitted by this EULA or required by applicable law on a non-excludable basis, any license granted under this Clause 3 shall be subject to the following prohibitions:

- the User must not sell, resell, rent, lease, loan, supply, publish, distribute, or redistribute the Software.
- the User must not alter, edit, or adapt the Software; and
- the User must not decompile, de-obfuscate or reverse engineer, or attempt to decompile, de-obfuscate or reverse engineer, the Software.

4. Restrictions of use of the License Key

4.1 The Software will run under a commercial license only if the License Key is plugged into the computer where the Software is installed; if the License Key is disconnected, the Software will stop working.

4.2 The License Key will work only on the computer where it is used for the first time (i.e. it will be locked to this computer).

4.3 The License Key can be unlocked by the Licensor, so to be locked again to a new computer, maximum three times a year.

5. Restrictions of the Evaluation License

5.1 Under the Evaluation License, the User agrees to use the Software only for evaluation purposes.

5.2 The User cannot use/publish/distribute data generated by the Software in the period of time when the Evaluation License is in force unless the User purchases a Commercial License.

6. Updates and upgrades

6.1 Licensor may, in its sole discretion, provide Updates (hotfix, patch or minor version update) of the Software; the User is entitled to receive and run Updates of the Software during the Term.

6.2 Licensor may, in its sole discretion, provide Upgrades (major version upgrade) of the Software; in order to be entitled to receive and run Upgrades of the Software, the User must subscribe a separate upgrade agreement.

7. Source Code

7.1 Nothing in this EULA shall give to the User or any other person any right to access or use the Source Code or constitute any license of the Source Code.

8. No assignment of Intellectual Property Rights

8.1 Nothing in this EULA shall operate to assign or transfer any Intellectual Property Rights from the Licensor to the User, or from the User to the Licensor.

9. Warranties

9.1 The Licensor warrants to the User that it has the legal right and authority to enter into this EULA and to perform its obligations under the EULA.

9.2 The User warrants to the Licensor that it has the legal right and authority to enter into this EULA and to perform its obligations under the EULA.



9.3 All of the parties' warranties and representations in respect of the subject matter of this EULA are expressly set out in this EULA. To the maximum extent permitted by applicable law, no other warranties or representations concerning the subject matter of this EULA will be implied into the EULA or any related contract.

10. Acknowledgements and warranty limitations

10.1 The User acknowledges that complex Software is never wholly free from defects, errors, and bugs; and subject to the other provisions of this EULA, the Licensor gives no warranty or representation that the Software will be wholly free from defects, errors, and bugs.

10.2 The User acknowledges that complex Software is never entirely free from security vulnerabilities; and subject to the other provisions of this EULA, the Licensor gives no warranty or representation that the Software will be entirely secure.

10.3 The User acknowledges that the Software is only designed to be compatible with that Software specified as compatible in the Software Specification; and the Licensor does not warrant or represent that the Software will be compatible with any other Software.

10.4 The User acknowledges that the Licensor will not provide any legal, financial, accountancy or taxation advice under this EULA or in relation to the Software; and, except to the extent expressly provided otherwise in this EULA, the Licensor does not warrant or represent that the Software or the use of the Software by the User will not give rise to any legal liability on the part of the User or any other person.

10.5 The User acknowledges that is fully responsible of protecting the License Key against loss and damage; in case of malfunction, the User will be entitled to obtain a replacement License Key only if the original defective License Key is returned to the Licensor by a trackable courier service; when the malfunction of the License Key is due by the User, the User will be charged of a cost of 80 EUR plus shipping cost for the replacement.

11. Limitations and exclusions of liability

11.1 Nothing in this EULA will:

- limit or exclude any liability for death or personal injury resulting from negligence.
- limit or exclude any liability for fraud or fraudulent misrepresentation.
- limit any liabilities in any way that is not permitted under applicable law; or
- exclude any liabilities that may not be excluded under applicable law,

and, if a party is a consumer, that party's statutory rights will not be excluded or limited by the EULA, except to the extent permitted by law.

11.2 The limitations and exclusions of liability set out in this Clause 11 and elsewhere in this EULA:

1. are subject to Clauses 11.1 and 14.6; and
2. govern all liabilities arising under the EULA or relating to the subject matter of the EULA, including liabilities arising in contract, in tort (including negligence) and for breach of statutory duty, except to the extent expressly provided otherwise in the EULA.

11.3 The Licensor will not be liable to the User in respect of any losses arising out of a Force Majeure Event.

11.4 The Licensor will not be liable to the User in respect of any loss of profits or anticipated savings.

11.5 The Licensor will not be liable to the User in respect of any loss of revenue or income.

11.6 The Licensor will not be liable to the User in respect of any loss of business, contracts, or opportunities.

11.7 The Licensor will not be liable to the User in respect of any loss or corruption of any data, database, or Software.

11.8 The Licensor will not be liable to the User in respect of any special, indirect, or consequential loss or damage.

11.9 The liability of the Licensor to the User under this EULA in respect of any event or series of related events shall not exceed the greater of:



- 1 EUR; and
- the total amount paid and payable by the User to the Licensor under the EULA in the 12 months period preceding the commencement of the event or events.

11.10 The aggregate liability of the Licensor to the User under this EULA shall not exceed the greater of:

- 1 EUR; and
- the total amount paid and payable by the User to the Licensor under the EULA.

12. Termination

12.1 Either party may terminate this EULA immediately by giving written notice of termination to the other party if the other party commits any breach of the EULA.

12.2 Either party may terminate this EULA immediately by giving written notice of termination to the other party if:

- the other party:
 1. is dissolved.
 2. ceases to conduct all (or substantially all) of its business.
 3. is or becomes unable to pay its debts as they fall due.
 4. is or becomes insolvent or is declared insolvent; or
 5. convenes a meeting or makes or proposes to make any arrangement or composition with its creditors.
- an administrator, administrative receiver, liquidator, receiver, trustee, manager or similar is appointed over any of the assets of the other party.
- an order is made for the winding up of the other party, or the other party passes a resolution for its winding up (other than for the purpose of a solvent company reorganization where the resulting entity will assume all the obligations of the other party under the EULA).
- if that other party is an individual:
 1. that other party dies.
 2. as a result of illness or incapacity, that other party becomes incapable of managing his or her own affairs; or
 3. that other party is the subject of a bankruptcy petition or order.

12.3 The Licensor may terminate this EULA immediately by giving written notice to the User if:

- any amount due to be paid by the User to the Licensor under the EULA is unpaid by the due date and remains unpaid upon the date that that written notice of termination is given; and
- the Licensor has given to the User at least 30 days' written notice, following the failure to pay, of its intention to terminate the EULA in accordance with this Clause 12.

13. Effects of termination

13.1 Upon the termination of this EULA, all of the provisions of this EULA shall cease to have effect, save that the following provisions of this EULA shall survive and continue to have effect (in accordance with their express terms or otherwise indefinitely): Clauses 1, 3.1, 11, 13, 14, 15.

13.2 The termination of this EULA shall not affect the accrued rights of either party.

13.3 For the avoidance of doubt, the licenses of the Software in this EULA shall terminate upon the termination of this EULA; and, accordingly, the User must immediately cease to use the Software upon the termination of this EULA.

13.4 Within 10 Business Days following the termination of this EULA, the User must:

- return to the Licensor or dispose of as the Licensor may instruct all media in its possession or control containing the Software; and
- irrevocably delete from all computer systems in its possession or control all copies of the Software.

14. General

14.1 No breach of any provision of this EULA shall be waived except with the express written consent of the party not in breach.

14.2 If any provision of this EULA is determined by any court or other competent authority to be unlawful and/or unenforceable, the other provisions of the EULA will continue in effect. If any unlawful and/or unenforceable provision would be lawful or enforceable if part of it were deleted, that part will be deemed to be deleted, and the rest of the provision will continue in effect (unless that would contradict the clear intention of the parties, in which case the entirety of the relevant provision will be deemed to be deleted).

14.3 This EULA may not be varied except by a written document signed by or on behalf of each of the parties.

14.4 Neither party may without the prior written consent of the other party assign, transfer, charge, license or otherwise deal in or dispose of any contractual rights or obligations under this EULA.

14.5 This EULA is made for the benefit of the parties, and is not intended to benefit any third party or be enforceable by any third party. The rights of the parties to terminate, rescind, or agree any amendment, waiver, variation, or settlement under or relating to this EULA are not subject to the consent of any third party.

14.6 Nothing in this EULA shall exclude or limit any liability of a party for fraud or fraudulent misrepresentation, or any other liability of a party that may not be excluded or limited under applicable law.

14.7 Subject to Clauses 11.1 and 14.6, this EULA shall constitute the entire agreement between the parties in relation to the subject matter of this EULA, and shall supersede all previous agreements, arrangements, and understandings between the parties in respect of that subject matter.

14.8 This EULA shall be governed by and construed in accordance with Italian law.

14.9 The courts of justice of Pisa - Italy shall have exclusive jurisdiction to adjudicate any dispute arising under or in connection with this EULA.

15. Interpretation

15.1 In this EULA, a reference to a statute or statutory provision includes a reference to:

- that statute or statutory provision as modified, consolidated, and/or re-enacted from time to time; and
- any subordinate legislation made under that statute or statutory provision.

15.2 The Clause headings do not affect the interpretation of this EULA.

15.3 In this EULA, general words shall not be given a restrictive interpretation by reason of being preceded or followed by words indicating a particular class of acts, matters or things.

16. Privacy Policy

16.1 By agreeing to be bound by this EULA, you hereby acknowledge that you are familiar with and agree to the terms of the Licensor's Privacy Policy available at <http://www.quipu.eu/privacy-policy/>.

16.2 This document is not the official document of Privacy Policy of the Licensor. For further information, please see the Privacy Policy in the footer of the Licensor's website.

16.3 The Licensor collects User information to communicate with User about the Licensor's products, services, and promotions. Personal data are also collected by the Licensor for the Software evaluation license and the Software activation license. The Licensor does not sell or rent User's personal information to third parties. The Licensor does, however, share User's information with third parties that provide services on Licensor's behalf or with whom the Licensor has partnered to offer a particular product or service.

16.4 Personal data collected are also needed for the Licensor to guarantee traceability of the medical device.

16.5 If the Licensor privacy policy changes, the Licensor shall post an updated version on Licensor's website. The policy revision date will be posted at the top of the page.



16.6 It is important to inform you that you are the only owner and responsible of data collected by your instance of the Software. These data may include personal data of the analyzed subjects that shall be managed according to the GDPR regulation <https://gdpr-info.eu/>.

15.3 Privacy policy

Document number: LEG0003EN rev. 9 of July 1st, 2020

Quipu s.r.l. is committed to safeguarding the privacy of our customers and website visitors; this policy sets out how we will treat your personal information.

Our website uses cookies. By using our website and agreeing to this policy, you consent to our use of cookies in accordance with the terms of this policy.

1. What information do we collect?

We may collect, store, and use the following kinds of personal information:

- a. information that you provide to us when you purchase one of our products (including Name, Company, Address, Email, Phone number).
- b. information relating to any transactions carried out between you and us, including information relating to any purchases you make of our goods or services.
- c. information that you provide to us for the purpose of using our free trial software (including Name, Company, Address, Email, Phone number, City, State, Country).
- d. information that you provide to us for the purpose of get an evaluation license (including First Name, Last Name, Company, Address, Email, Phone number, City, State, Country).
- e. information that you provide to us for the purpose of activate license (including First Name, Last Name, Company, Address, Email, Phone number, City, State, Country).
- f. information about your computer and about your visits to and use of our website (including your IP address, geographical location, browser type and version, operating system, referral source, length of visit, page views, website navigation).
- g. information that you provide to us when you visit the "Contact us" section on the website to have further information (including Name, Email and Phone number)
- h. any other information that you choose to send to us.

Before you disclose to us the personal information of another person, you must obtain that person's consent to both the disclosure and the processing of that personal information in accordance with the terms of this privacy policy.

2. Why we collect your personal data

We ask you to share your personal data with us for purposes that include, but are not limited to:

- Activating or registering licenses for QUIPU's product or enabling functionalities.
- Receiving information about QUIPU's product and services.
- Participating in QUIPU online communities, including our social media channels/pages and blogs.
- Helping us to improve the product and services, and allowing QUIPU to keep you informed of new versions of the software.
- Resolving consumer and/or product and services issues.
- Managing customer relationships.
- Facilitating information access.
- Enhancing communications.
- Traceability of medical device.

We generally process your personal data only for those purposes that we have communicated to you. If we use it for other (closely related) purposes, additional data protection measures will be implemented if required by law.

3. Definitions for personal data processing

**User**

The individual using this Application, which must coincide with or be authorized by the Data Subject, to whom the Personal Data refer.

Data Subject

The legal or natural person to whom the Personal Data refers.

Data Processor (or Data Supervisor)

The natural person, legal person, public administration or any other body, association or organization authorized by the Data Controller to process the Personal Data in compliance with this privacy policy.

Data Controller (or Owner)

The natural person, legal person, public administration or any other body, association or organization with the right, also jointly with another Data Controller, to make decisions regarding the purposes, and the methods of processing of Personal Data and the means used, including the security measures concerning the operation and use of this Application. The Data Controller, unless otherwise specified, is the Owner of this Application.

Referring Person of Personal Data Processing

The natural person that the CEO of the Company nominates as a person who acts as an Internal Referring Person for processing personal data. This person is nominated after a verification of his/her competencies and abilities in Personal Data Processing and related legal issues.

This Application

The hardware or software tool by which the Personal Data of the User is collected.

Legal information

Notice to European Users: this privacy statement has been prepared in fulfillment of the obligations under Art. 10 of EC Directive n. 95/46/EC, and under the provisions of Directive 2002/58/EC, as revised by Directive 2009/136/EC, on the subject of Cookies. It has also been prepared in fulfillment of the obligations of the General Data Protection Regulation (GDPR) (EU) 2016/679.

This privacy policy relates solely to this Application.

4. Contact data**Data controller's personal data:**

- Name: Vincenzo Gemignani
- Address: Via Verdi 3/b, Torre del Lago (LU)
- Email: gemignani@quipu.eu
- PEC: vincenzo.gemignani@pec.it
- Phone number: 0039/050-3152612

Referring Person of Personal Data Processing's personal data:

- Name: Elisabetta Bianchini
- Address: via Nottolini 466, San Concordio (LU)
- Email: bianchini@quipu.eu
- PEC: elisabettabianchini@pec.it
- Phone number: 0039/050-3152630

5. Methods of processing

The Data Controller processes the Data of Users in a proper manner and shall take appropriate security measures to prevent unauthorized access, disclosure, modification, or unauthorized destruction of the Data. The Data processing is carried out using computers and/or IT enabled tools, following organizational procedures and modes strictly related to the purposes indicated. In addition to the Data Controller, in some cases, the Data may be accessible to certain types of persons in charge, involved with the operation of the site (administration, sales, marketing, legal, system administration) or external parties (such as third party technical service providers, mail carriers, hosting providers, IT companies, communications agencies) appointed, if necessary, as Data Processors by the Owner. The updated list of these parties may be requested from the Data Controller at any time.

6. **Place**

Personal data are processed at the Data Controller's operating offices and in any other places where the parties involved with the processing are located. For further information, please contact the Data Controller at privacy@quipu.eu.

7. **Retention time**

Personal data are kept for the time necessary to provide the service requested by the User that is estimated to be 10 years; the User can always request that the Data Controller suspend or remove the data, sending an email at privacy@quipu.eu.

8. **Cookies**

A cookie is a file containing an identifier (a string of letters and numbers) that is sent by a web server to a web browser and is stored by the browser. The identifier is then sent back to the server each time the browser requests a page from the server. This enables the web server to identify and track the web browser. We may use both "session" cookies and "persistent" cookies on the website. Session cookies will be deleted from your computer when you close your browser. Persistent cookies will remain stored on your computer until deleted, or until they reach a specified expiry date.

While browsing our website you may also receive cookies from third parties such as those used for Google Analytics, a web analysis service supplied by Google, Inc. ("Google"). We use Google Analytics to analyze the use of our website. Google Analytics generates statistical and other information about website use by means of cookies, which are stored on users' computers. The information generated relating to our website is used to create reports about the use of the website. Google will store this information. Google's privacy policy is available at: <http://www.google.com/privacypolicy.html>.

Most browsers allow you to reject all cookies, whilst some browsers allow you to reject just third party cookies. For example, in Internet Explorer (version 9) you can refuse all cookies by clicking "Tools", "Internet options", "Privacy", and selecting "Block All Cookies" using the sliding selector. Blocking all cookies will, however, have a negative impact upon the usability of many websites.

There are a number of different ways of managing cookies; please refer to the instruction manual or help screen of your browser to determine how to control and adjust settings. Users may change the predefined configuration and disable cookies (block them permanently) by setting the highest level of protection.

Below are the paths to follow to manage cookies on the following browsers:

Explorer:

<https://support.microsoft.com/en-gb/help/17442/windows-internet-explorer-delete-manage-cookies>

Safari:

https://support.apple.com/kb/PH21411?viewlocale=en_US&locale=en_US

Chrome:

<https://support.google.com/chrome/answer/95647?hl=it&hlrm=fr&hlrm=en>

Firefox:

<http://support.mozilla.org/it-IT/kb/enable-and-disable-cookies-website-preferences>

How to disable third party services' cookies:

Google Analytics services:

<http://www.google.it/analytics/learn/privacy.html>

<https://tools.google.com/dlpage/gaoptout>

Third party cookies are not controlled directly by the Data Controller, and so if you wish to revoke your consent to use of these cookies you must contact the third parties' internet sites or go to the website www.youronlinechoices.com to obtain information on how to delete or manage cookies on the basis of the browser you use and to manage your preferences regarding third-party profiling cookies.

In accordance with section 122 paragraph two of Legislative Decree 196/2003 and following simplified methods for notification and acquisition of consent to use of cookies published in Gazzetta Ufficiale no. 126 on June 3 2014 and the corresponding register of measures no. 229 dated May 8 2014, at the foot of each page of QUIPU website it is possible to find the link to cookies in the Privacy Policy document.

9. **Using your personal information**



Personal information submitted to us will be used for the purposes specified in this privacy policy or in relevant parts of the website.

We may use your personal information to:

- a. medical device traceability;
- b. send you e-mail invitation in product usability surveys.
- c. keep you posted on last products' updates.
- d. send statements and invoices to you, and collect payments from you.
- e. send you general commercial communications.
- f. send you email notifications which you have specifically requested.
- g. administer the website.
- h. improve your browsing experience by personalizing our website.
- i. enable your use of the services available on our website.
- j. send you goods purchased via the website, and supply to you services purchased via the website.
- k. deal with enquiries and complaints made by or about you relating to our website.
- l. keep the website secure and prevent fraud.
- m. set up your free trial software license.
- n. set up your license activation.

We will not, without your express consent, provide your personal information to any third parties for the purpose of direct marketing.

10. Duration of Data Processing

The duration of data processing is balanced with the scope of the processing itself. It is limited to the services required by the customers. You can request for restriction or suspension of the processing by sending an email at privacy@quipu.eu.

11. Personal data provision

Your consent to processing of personal data is mandatory for the Company for the reasons listed in section 2, especially for the traceability of the medical device sold by the Company. If you do not agree with this consent, it will not be possible to download Company's product or activate any evaluation/activation license.

12. How to propose requests for Personal Data

If you desire to modify, get access, ask for erasure or rectification, or any other request related to your personal data provided, it is necessary to send an email to privacy@quipu.eu specifying your request. The Data protection Officer or the controller will perform your request and reply to your mail.

13. Disclosures

We may disclose your personal information to any of our employees, officers, agents, suppliers, or subcontractors insofar as reasonably necessary for the purposes set out in this privacy policy. In addition, we may disclose your personal information:

1. to the extent that we are required to do so by law.
2. in connection with any ongoing or prospective legal proceedings.
3. in order to establish, exercise or defend our legal rights (including providing information to others for the purposes of fraud prevention and reducing credit risk).

Except as provided in this privacy policy, we will not provide your information to third parties.

14. International data transfer

Information that we collect may be stored and processed in and transferred between any of the countries in which we operate in order to enable us to use the information in accordance with this privacy policy.

Information which you provide may be transferred to countries (including the United States and Canada) which do not have data protection laws equivalent to those in force in the European Economic Area.

You expressly agree to such transfers of personal information.

15. Security of your personal information



We will take reasonable technical and organizational precautions to prevent the loss, misuse, or alteration of your personal information.

We will store all the personal information you provide on our secure (password- and firewall-protected) servers.

All electronic transactions entered into via the website will be protected by encryption technology.

You acknowledge that the transmission of information over the internet is inherently insecure, and we cannot guarantee the security of data sent over the internet.

QUIPU's activities also include ultrasound images analysis for third parties. Images provided by the customer to Quipu should be in an anonymous form. Quipu, if required by the customer, can provide a cryptographic process to ensure data security.

16. Personal data breach

In case of a personal data breach, QUIPU carries out specific actions in accordance with Regulation (EU) 2016/679 (General Data Protection Regulation). QUIPU shall without undue delay and, where feasible, not later than 72 hours after having become aware of it, notify the personal data breach to the supervisory authority competent in accordance with Article 55 of GDPR, unless the personal data breach is unlikely to result in a risk to the rights and freedoms of natural persons. Where the notification to the supervisory authority is not made within 72 hours, it shall be accompanied by reasons for the delay.

Article 32 of GDPR indicates that QUIPU shall implement appropriate technical and organizational measures to ensure a level of security appropriate to the risk.

17. Policy amendments

We may update this privacy policy from time to time by posting a new version on our website. You should check this page occasionally to ensure you are happy with any changes.

18. Your rights

A data subject shall have the right to obtain confirmation as to whether or not personal data concerning him exist and to know their content and origin, to check their accuracy and to request integration or updating, or rectification (section 7 of Legislative Decree no. 196/2003) or objection to data processing, as stated in Article 21 of GDPR. Your rights are listed here:

- Article 12: Transparent information, communication and modalities for the exercise of the rights of the data subject
- Article 13: Information to be provided where personal data are collected from the data subject
- Article 14: Information to be provided where personal data have not been obtained from the data subject
- Article 15: Right of access by the data subject
- Article 16: Right to rectification
- Article 17: Right to erasure ('right to be forgotten')
- Article 18: Right to restriction of processing
- Article 19: Notification obligation regarding rectification or erasure of personal data or restriction of processing
- Article 20: Right to data portability
- Article 21: Right to object
- Article 22: Automated individual decision-making, including profiling

Under the same section, data subjects are entitled to request erasure, anonymization or blocking of data that have been processed unlawfully, and in all cases to object to their treatment on legitimate grounds.

Requests in this regard should be sent to the Data Controller, sending an email at privacy@quipu.eu.

We may withhold such personal information to the extent permitted by law.

You can expressly agree to our use of your personal information for marketing purposes; you can opt out of the use of your personal information for marketing purposes by sending an email to us at privacy@quipu.eu.

19. Third party websites

The website contains links to other websites. We are not responsible for the privacy policies or practices of third party websites.

We may provide only your email address to third party websites in order to set up a survey about our services and products. The email address will be used only to send the invitation to our surveys. Every kind of sensitive information given to the survey provider are treated as an aggregate variable so both Quipu and



any eventual third part involved in surveys don't retain anything except of what explained in section Cookies.

It is in count that joining any kind of survey powered by a third part you also accept the private policy of the third part.

We are not responsible of the eventual wrongs belonging to the third part.

20. Updating information

Please let us know if the personal information which we hold about you needs to be corrected or updated. You can send an email to privacy@quipu.eu specifying your request.

21. Changes to this Privacy Policy

The Data Controller reserves the right to make changes to this privacy policy at any time by giving notice to its Users on the website. It is strongly recommended to check this page often, referring to the date of the last modification listed at the bottom. If a User objects to any of the changes to the Policy, the User must cease using this Application and can request that the Data Controller removes the Personal Data. Unless stated otherwise, the then-current privacy policy applies to all Personal Data the Data Controller has about Users.

22. Contacts

If you have any questions about this privacy policy or our treatment of your personal information, please write to us by email to privacy@quipu.eu or by post to Quipu s.r.l., via Moruzzi 1, Pisa I-56124, Italy.

23. Data controller

The data controller responsible in respect of the information collected on this website is Vincenzo Gemignani, Via Verdi 3/b, Torre del Lago (LU), Italy.

15.4 Open source

This page contains Third Party Software Notices and/or Additional Terms and Conditions for licensed third party software components included within Cardiovascular Suite software products.

The Qt Toolkit Copyright © The Qt Company Ltd. and other contributors

Qt is available under the GNU Lesser General Public License version 3.

The Qt Toolkit is Copyright (C) 2018 The Qt Company Ltd. and other contributors.

Contact: <https://www.qt.io/licensing/>

FFmpeg Copyright © Fabrice Bellard and FFMpeg Team

Modified sources: <https://github.com/Quipusrl/FFmpeg>

FFmpeg is free software; you can redistribute it and/or modify it under the terms of the GNU Lesser General Public License as published by the Free Software Foundation; either version 2.1 of the License, or (at your option) any later version.

FFmpeg is distributed in the hope that it will be useful, but WITHOUT ANY WARRANTY; without even the implied warranty of MERCHANTABILITY or FITNESS FOR A PARTICULAR PURPOSE. See the GNU Lesser General Public License for more details.

You should have received a copy of the GNU Lesser General Public License along with FFMpeg; if not, write to the Free Software Foundation, Inc., 51 Franklin Street, Fifth Floor, Boston, MA 02110-1301 USA

QtAV Copyright © Wang Bin

Modified sources: <https://github.com/Quipusrl/QtAV>



QtAV is free software; you can redistribute it and/or modify it under the terms of the GNU Lesser General Public License as published by the Free Software Foundation; either version 2.1 of the License, or (at your option) any later version.

QtAV is distributed in the hope that it will be useful, but WITHOUT ANY WARRANTY; without even the implied warranty of MERCHANTABILITY or FITNESS FOR A PARTICULAR PURPOSE. See the GNU Lesser General Public License for more details.

You should have received a copy of the GNU Lesser General Public License along with QtAV; if not, write to the Free Software Foundation, Inc., 51 Franklin Street, Fifth Floor, Boston, MA 02110-1301 USA

7-Zip Extra Copyright © Igor Pavlov

7-Zip Extra files are under the GNU LGPL license. You can use 7-Zip Extra on any computer, including a computer in a commercial organization. You don't need to register or pay for 7-Zip.

Contact: <https://www.7-zip.org>

15.5 LGPL 2.1

GNU LESSER GENERAL PUBLIC LICENSE

Version 2.1, February 1999

Copyright (C) 1991, 1999 Free Software Foundation, Inc.
51 Franklin Street, Fifth Floor, Boston, MA 02110-1301 USA

Everyone is permitted to copy and distribute verbatim copies of this license document, but changing it is not allowed.

[This is the first released version of the Lesser GPL. It also counts as the successor of the GNU Library Public License, version 2, hence the version number 2.1.]

Preamble

The licenses for most software are designed to take away your freedom to share and change it. By contrast, the GNU General Public Licenses are intended to guarantee your freedom to share and change free software--to make sure the software is free for all its users.

This license, the Lesser General Public License, applies to some specially designated software packages--typically libraries--of the Free Software Foundation and other authors who decide to use it. You can use it too, but we suggest you first think carefully about whether this license or the ordinary General Public License is the better strategy to use in any particular case, based on the explanations below.

When we speak of free software, we are referring to freedom of use, not price. Our General Public Licenses are designed to make sure that you have the freedom to distribute copies of free software (and charge for this service if you wish); that you receive source code or can get it if you want it; that you can change the software and use pieces of it in new free programs; and that you are informed that you can do these things.

To protect your rights, we need to make restrictions that forbid distributors to deny you these rights or to ask you to surrender these rights. These restrictions translate to certain responsibilities for you if you distribute copies of the library or if you modify it.

For example, if you distribute copies of the library, whether gratis or for a fee, you must give the recipients all the rights that we gave you. You must make sure that they, too, receive or can get the source code. If you link other code with the library, you must provide complete object files to the recipients, so that they can relink them with the library after making changes to the library and recompiling it. And you must show them these terms so they know their rights.



We protect your rights with a two-step method: (1) we copyright the library, and (2) we offer you this license, which gives you legal permission to copy, distribute and/or modify the library.

To protect each distributor, we want to make it very clear that there is no warranty for the free library. Also, if the library is modified by someone else and passed on, the recipients should know that what they have is not the original version, so that the original author's reputation will not be affected by problems that might be introduced by others.

Finally, software patents pose a constant threat to the existence of any free program. We wish to make sure that a company cannot effectively restrict the users of a free program by obtaining a restrictive license from a patent holder. Therefore, we insist that any patent license obtained for a version of the library must be consistent with the full freedom of use specified in this license.

Most GNU software, including some libraries, is covered by the ordinary GNU General Public License. This license, the GNU Lesser General Public License, applies to certain designated libraries, and is quite different from the ordinary General Public License. We use this license for certain libraries in order to permit linking those libraries into non-free programs.

When a program is linked with a library, whether statically or using a shared library, the combination of the two is legally speaking a combined work, a derivative of the original library. The ordinary General Public License therefore permits such linking only if the entire combination fits its criteria of freedom. The Lesser General Public License permits more lax criteria for linking other code with the library.

We call this license the "Lesser" General Public License because it does Less to protect the user's freedom than the ordinary General Public License. It also provides other free software developers Less of an advantage over competing non-free programs. These disadvantages are the reason we use the ordinary General Public License for many libraries. However, the Lesser license provides advantages in certain special circumstances.

For example, on rare occasions, there may be a special need to encourage the widest possible use of a certain library, so that it becomes a de-facto standard. To achieve this, non-free programs must be allowed to use the library. A more frequent case is that a free library does the same job as widely used non-free libraries. In this case, there is little to gain by limiting the free library to free software only, so we use the Lesser General Public License.

In other cases, permission to use a particular library in non-free programs enables a greater number of people to use a large body of free software. For example, permission to use the GNU C Library in non-free programs enables many more people to use the whole GNU operating system, as well as its variant, the GNU/Linux operating system.

Although the Lesser General Public License is Less protective of the users' freedom, it does ensure that the user of a program that is linked with the Library has the freedom and the wherewithal to run that program using a modified version of the Library.

The precise terms and conditions for copying, distribution and modification follow. Pay close attention to the difference between a "work based on the library" and a "work that uses the library". The former contains code derived from the library, whereas the latter must be combined with the library in order to run.

TERMS AND CONDITIONS FOR COPYING, DISTRIBUTION AND MODIFICATION

0. This License Agreement applies to any software library or other program which contains a notice placed by the copyright holder or other authorized party saying it may be distributed under the terms of this Lesser General Public License (also called "this License"). Each licensee is addressed as "you".

A "library" means a collection of software functions and/or data prepared so as to be conveniently linked with application programs (which use some of those functions and data) to form executables.

The "Library", below, refers to any such software library or work which has been distributed under these terms. A "work based on the Library" means either the Library or any derivative work under copyright law: that is to say, a work containing the Library or a portion of it, either verbatim or with modifications and/or translated straightforwardly into another language. (Hereinafter, translation is included without limitation in the term "modification".)



"Source code" for a work means the preferred form of the work for making modifications to it. For a library, complete source code means all the source code for all modules it contains, plus any associated interface definition files, plus the scripts used to control compilation and installation of the library.

Activities other than copying, distribution and modification are not covered by this License; they are outside its scope. The act of running a program using the Library is not restricted, and output from such a program is covered only if its contents constitute a work based on the Library (independent of the use of the Library in a tool for writing it). Whether that is true depends on what the Library does and what the program that uses the Library does.

1. You may copy and distribute verbatim copies of the Library's complete source code as you receive it, in any medium, provided that you conspicuously and appropriately publish on each copy an appropriate copyright notice and disclaimer of warranty; keep intact all the notices that refer to this License and to the absence of any warranty; and distribute a copy of this License along with the Library.

You may charge a fee for the physical act of transferring a copy, and you may at your option offer warranty protection in exchange for a fee.

2. You may modify your copy or copies of the Library or any portion of it, thus forming a work based on the Library, and copy and distribute such modifications or work under the terms of Section 1 above, provided that you also meet all of these conditions:

- **a)** The modified work must itself be a software library.
- **b)** You must cause the files modified to carry prominent notices stating that you changed the files and the date of any change.
- **c)** You must cause the whole of the work to be licensed at no charge to all third parties under the terms of this License.
- **d)** If a facility in the modified Library refers to a function or a table of data to be supplied by an application program that uses the facility, other than as an argument passed when the facility is invoked, then you must make a good faith effort to ensure that, in the event an application does not supply such function or table, the facility still operates, and performs whatever part of its purpose remains meaningful.

(For example, a function in a library to compute square roots has a purpose that is entirely well-defined independent of the application. Therefore, Subsection 2d requires that any application-supplied function or table used by this function must be optional: if the application does not supply it, the square root function must still compute square roots.)

These requirements apply to the modified work as a whole. If identifiable sections of that work are not derived from the Library, and can be reasonably considered independent and separate works in themselves, then this License, and its terms, do not apply to those sections when you distribute them as separate works. But when you distribute the same sections as part of a whole which is a work based on the Library, the distribution of the whole must be on the terms of this License, whose permissions for other licensees extend to the entire whole, and thus to each and every part regardless of who wrote it.

Thus, it is not the intent of this section to claim rights or contest your rights to work written entirely by you; rather, the intent is to exercise the right to control the distribution of derivative or collective works based on the Library.

In addition, mere aggregation of another work not based on the Library with the Library (or with a work based on the Library) on a volume of a storage or distribution medium does not bring the other work under the scope of this License.

3. You may opt to apply the terms of the ordinary GNU General Public License instead of this License to a given copy of the Library. To do this, you must alter all the notices that refer to this License, so that they refer to the ordinary GNU General Public License, version 2, instead of to this License. (If a newer version than version 2 of the ordinary GNU General Public License has appeared, then you can specify that version instead if you wish.) Do not make any other change in these notices.



Once this change is made in a given copy, it is irreversible for that copy, so the ordinary GNU General Public License applies to all subsequent copies and derivative works made from that copy.

This option is useful when you wish to copy part of the code of the Library into a program that is not a library.

4. You may copy and distribute the Library (or a portion or derivative of it, under Section 2) in object code or executable form under the terms of Sections 1 and 2 above provided that you accompany it with the complete corresponding machine-readable source code, which must be distributed under the terms of Sections 1 and 2 above on a medium customarily used for software interchange.

If distribution of object code is made by offering access to copy from a designated place, then offering equivalent access to copy the source code from the same place satisfies the requirement to distribute the source code, even though third parties are not compelled to copy the source along with the object code.

5. A program that contains no derivative of any portion of the Library, but is designed to work with the Library by being compiled or linked with it, is called a "work that uses the Library". Such a work, in isolation, is not a derivative work of the Library, and therefore falls outside the scope of this License.

However, linking a "work that uses the Library" with the Library creates an executable that is a derivative of the Library (because it contains portions of the Library), rather than a "work that uses the library". The executable is therefore covered by this License. Section 6 states terms for distribution of such executables.

When a "work that uses the Library" uses material from a header file that is part of the Library, the object code for the work may be a derivative work of the Library even though the source code is not. Whether this is true is especially significant if the work can be linked without the Library, or if the work is itself a library. The threshold for this to be true is not precisely defined by law.

If such an object file uses only numerical parameters, data structure layouts and accessors, and small macros and small inline functions (ten lines or less in length), then the use of the object file is unrestricted, regardless of whether it is legally a derivative work. (Executables containing this object code plus portions of the Library will still fall under Section 6.)

Otherwise, if the work is a derivative of the Library, you may distribute the object code for the work under the terms of Section 6. Any executables containing that work also fall under Section 6, whether or not they are linked directly with the Library itself.

6. As an exception to the Sections above, you may also combine or link a "work that uses the Library" with the Library to produce a work containing portions of the Library, and distribute that work under terms of your choice, provided that the terms permit modification of the work for the customer's own use and reverse engineering for debugging such modifications.

You must give prominent notice with each copy of the work that the Library is used in it and that the Library and its use are covered by this License. You must supply a copy of this License. If the work during execution displays copyright notices, you must include the copyright notice for the Library among them, as well as a reference directing the user to the copy of this License. Also, you must do one of these things:

- **a)** Accompany the work with the complete corresponding machine-readable source code for the Library including whatever changes were used in the work (which must be distributed under Sections 1 and 2 above); and, if the work is an executable linked with the Library, with the complete machine-readable "work that uses the Library", as object code and/or source code, so that the user can modify the Library and then relink to produce a modified executable containing the modified Library. (It is understood that the user who changes the contents of definitions files in the Library will not necessarily be able to recompile the application to use the modified definitions.)
- **b)** Use a suitable shared library mechanism for linking with the Library. A suitable mechanism is one that (1) uses at run time a copy of the library already present on the user's computer system, rather than copying library functions into the executable, and (2) will operate properly with a modified version of the library, if the user installs one, as long as the modified version is interface-compatible with the version that the work was made with.



- **c)** Accompany the work with a written offer, valid for at least three years, to give the same user the materials specified in Subsection 6a, above, for a charge no more than the cost of performing this distribution.
- **d)** If distribution of the work is made by offering access to copy from a designated place, offer equivalent access to copy the above specified materials from the same place.
- **e)** Verify that the user has already received a copy of these materials or that you have already sent this user a copy.

For an executable, the required form of the "work that uses the Library" must include any data and utility programs needed for reproducing the executable from it. However, as a special exception, the materials to be distributed need not include anything that is normally distributed (in either source or binary form) with the major components (compiler, kernel, and so on) of the operating system on which the executable runs, unless that component itself accompanies the executable.

It may happen that this requirement contradicts the license restrictions of other proprietary libraries that do not normally accompany the operating system. Such a contradiction means you cannot use both them and the Library together in an executable that you distribute.

7. You may place library facilities that are a work based on the Library side-by-side in a single library together with other library facilities not covered by this License, and distribute such a combined library, provided that the separate distribution of the work based on the Library and of the other library facilities is otherwise permitted, and provided that you do these two things:

- **a)** Accompany the combined library with a copy of the same work based on the Library, uncombined with any other library facilities. This must be distributed under the terms of the Sections above.
- **b)** Give prominent notice with the combined library of the fact that part of it is a work based on the Library, and explaining where to find the accompanying uncombined form of the same work.

8. You may not copy, modify, sublicense, link with, or distribute the Library except as expressly provided under this License. Any attempt otherwise to copy, modify, sublicense, link with, or distribute the Library is void, and will automatically terminate your rights under this License. However, parties who have received copies, or rights, from you under this License will not have their licenses terminated so long as such parties remain in full compliance.

9. You are not required to accept this License, since you have not signed it. However, nothing else grants you permission to modify or distribute the Library or its derivative works. These actions are prohibited by law if you do not accept this License. Therefore, by modifying or distributing the Library (or any work based on the Library), you indicate your acceptance of this License to do so, and all its terms and conditions for copying, distributing or modifying the Library or works based on it.

10. Each time you redistribute the Library (or any work based on the Library), the recipient automatically receives a license from the original licensor to copy, distribute, link with or modify the Library subject to these terms and conditions. You may not impose any further restrictions on the recipients' exercise of the rights granted herein. You are not responsible for enforcing compliance by third parties with this License.

11. If, as a consequence of a court judgment or allegation of patent infringement or for any other reason (not limited to patent issues), conditions are imposed on you (whether by court order, agreement or otherwise) that contradict the conditions of this License, they do not excuse you from the conditions of this License. If you cannot distribute so as to satisfy simultaneously your obligations under this License and any other pertinent obligations, then as a consequence you may not distribute the Library at all. For example, if a patent license would not permit royalty-free redistribution of the Library by all those who receive copies directly or indirectly through you, then the only way you could satisfy both it and this License would be to refrain entirely from distribution of the Library.

If any portion of this section is held invalid or unenforceable under any particular circumstance, the balance of the section is intended to apply, and the section as a whole is intended to apply in other circumstances.

It is not the purpose of this section to induce you to infringe any patents or other property right claims or to contest validity of any such claims; this section has the sole purpose of protecting the integrity of the free software distribution system which is implemented by public license practices. Many people have made generous



contributions to the wide range of software distributed through that system in reliance on consistent application of that system; it is up to the author/donor to decide if he or she is willing to distribute software through any other system and a licensee cannot impose that choice.

This section is intended to make thoroughly clear what is believed to be a consequence of the rest of this License.

12. If the distribution and/or use of the Library is restricted in certain countries either by patents or by copyrighted interfaces, the original copyright holder who places the Library under this License may add an explicit geographical distribution limitation excluding those countries, so that distribution is permitted only in or among countries not thus excluded. In such case, this License incorporates the limitation as if written in the body of this License.

13. The Free Software Foundation may publish revised and/or new versions of the Lesser General Public License from time to time. Such new versions will be similar in spirit to the present version, but may differ in detail to address new problems or concerns.

Each version is given a distinguishing version number. If the Library specifies a version number of this License which applies to it and "any later version", you have the option of following the terms and conditions either of that version or of any later version published by the Free Software Foundation. If the Library does not specify a license version number, you may choose any version ever published by the Free Software Foundation.

14. If you wish to incorporate parts of the Library into other free programs whose distribution conditions are incompatible with these, write to the author to ask for permission. For software which is copyrighted by the Free Software Foundation, write to the Free Software Foundation; we sometimes make exceptions for this. Our decision will be guided by the two goals of preserving the free status of all derivatives of our free software and of promoting the sharing and reuse of software generally.

NO WARRANTY

15. BECAUSE THE LIBRARY IS LICENSED FREE OF CHARGE, THERE IS NO WARRANTY FOR THE LIBRARY, TO THE EXTENT PERMITTED BY APPLICABLE LAW. EXCEPT WHEN OTHERWISE STATED IN WRITING THE COPYRIGHT HOLDERS AND/OR OTHER PARTIES PROVIDE THE LIBRARY "AS IS" WITHOUT WARRANTY OF ANY KIND, EITHER EXPRESSED OR IMPLIED, INCLUDING, BUT NOT LIMITED TO, THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. THE ENTIRE RISK AS TO THE QUALITY AND PERFORMANCE OF THE LIBRARY IS WITH YOU. SHOULD THE LIBRARY PROVE DEFECTIVE, YOU ASSUME THE COST OF ALL NECESSARY SERVICING, REPAIR OR CORRECTION.

16. IN NO EVENT UNLESS REQUIRED BY APPLICABLE LAW OR AGREED TO IN WRITING WILL ANY COPYRIGHT HOLDER, OR ANY OTHER PARTY WHO MAY MODIFY AND/OR REDISTRIBUTE THE LIBRARY AS PERMITTED ABOVE, BE LIABLE TO YOU FOR DAMAGES, INCLUDING ANY GENERAL, SPECIAL, INCIDENTAL OR CONSEQUENTIAL DAMAGES ARISING OUT OF THE USE OR INABILITY TO USE THE LIBRARY (INCLUDING BUT NOT LIMITED TO LOSS OF DATA OR DATA BEING RENDERED INACCURATE OR LOSSES SUSTAINED BY YOU OR THIRD PARTIES OR A FAILURE OF THE LIBRARY TO OPERATE WITH ANY OTHER SOFTWARE), EVEN IF SUCH HOLDER OR OTHER PARTY HAS BEEN ADVISED OF THE POSSIBILITY OF SUCH DAMAGES.

END OF TERMS AND CONDITIONS

15.6 LGPL 3

GNU LESSER GENERAL PUBLIC LICENSE

Version 3, 29 June 2007

Copyright © 2007 Free Software Foundation, Inc. <<https://fsf.org/>>

Everyone is permitted to copy and distribute verbatim copies of this license document, but changing it is not allowed.



This version of the GNU Lesser General Public License incorporates the terms and conditions of version 3 of the GNU General Public License, supplemented by the additional permissions listed below.

0. Additional Definitions.

As used herein, “this License” refers to version 3 of the GNU Lesser General Public License, and the “GNU GPL” refers to version 3 of the GNU General Public License.

“The Library” refers to a covered work governed by this License, other than an Application or a Combined Work as defined below.

An “Application” is any work that makes use of an interface provided by the Library, but which is not otherwise based on the Library. Defining a subclass of a class defined by the Library is deemed a mode of using an interface provided by the Library.

A “Combined Work” is a work produced by combining or linking an Application with the Library. The particular version of the Library with which the Combined Work was made is also called the “Linked Version”.

The “Minimal Corresponding Source” for a Combined Work means the Corresponding Source for the Combined Work, excluding any source code for portions of the Combined Work that, considered in isolation, are based on the Application, and not on the Linked Version.

The “Corresponding Application Code” for a Combined Work means the object code and/or source code for the Application, including any data and utility programs needed for reproducing the Combined Work from the Application, but excluding the System Libraries of the Combined Work.

1. Exception to Section 3 of the GNU GPL.

You may convey a covered work under sections 3 and 4 of this License without being bound by section 3 of the GNU GPL.

2. Conveying Modified Versions.

If you modify a copy of the Library, and, in your modifications, a facility refers to a function or data to be supplied by an Application that uses the facility (other than as an argument passed when the facility is invoked), then you may convey a copy of the modified version:

- a) under this License, provided that you make a good faith effort to ensure that, in the event an Application does not supply the function or data, the facility still operates, and performs whatever part of its purpose remains meaningful, or
- b) under the GNU GPL, with none of the additional permissions of this License applicable to that copy.

3. Object Code Incorporating Material from Library Header Files.

The object code form of an Application may incorporate material from a header file that is part of the Library. You may convey such object code under terms of your choice, provided that, if the incorporated material is not limited to numerical parameters, data structure layouts and accessors, or small macros, inline functions and templates (ten or fewer lines in length), you do both of the following:

- a) Give prominent notice with each copy of the object code that the Library is used in it and that the Library and its use are covered by this License.
- b) Accompany the object code with a copy of the GNU GPL and this license document.

4. Combined Works.

You may convey a Combined Work under terms of your choice that, taken together, effectively do not restrict modification of the portions of the Library contained in the Combined Work and reverse engineering for debugging such modifications, if you also do each of the following:

- a) Give prominent notice with each copy of the Combined Work that the Library is used in it and that the Library and its use are covered by this License.
- b) Accompany the Combined Work with a copy of the GNU GPL and this license document.



- c) For a Combined Work that displays copyright notices during execution, include the copyright notice for the Library among these notices, as well as a reference directing the user to the copies of the GNU GPL and this license document.
- d) Do one of the following:
 - 0) Convey the Minimal Corresponding Source under the terms of this License, and the Corresponding Application Code in a form suitable for, and under terms that permit, the user to recombine or relink the Application with a modified version of the Linked Version to produce a modified Combined Work, in the manner specified by section 6 of the GNU GPL for conveying Corresponding Source.
 - 1) Use a suitable shared library mechanism for linking with the Library. A suitable mechanism is one that (a) uses at run time a copy of the Library already present on the user's computer system, and (b) will operate properly with a modified version of the Library that is interface-compatible with the Linked Version.
- e) Provide Installation Information, but only if you would otherwise be required to provide such information under section 6 of the GNU GPL, and only to the extent that such information is necessary to install and execute a modified version of the Combined Work produced by recombining or relinking the Application with a modified version of the Linked Version. (If you use option 4d0, the Installation Information must accompany the Minimal Corresponding Source and Corresponding Application Code. If you use option 4d1, you must provide the Installation Information in the manner specified by section 6 of the GNU GPL for conveying Corresponding Source.)

5. Combined Libraries.

You may place library facilities that are a work based on the Library side by side in a single library together with other library facilities that are not Applications and are not covered by this License, and convey such a combined library under terms of your choice, if you do both of the following:

- a) Accompany the combined library with a copy of the same work based on the Library, uncombined with any other library facilities, conveyed under the terms of this License.
- b) Give prominent notice with the combined library that part of it is a work based on the Library, and explaining where to find the accompanying uncombined form of the same work.

6. Revised Versions of the GNU Lesser General Public License.

The Free Software Foundation may publish revised and/or new versions of the GNU Lesser General Public License from time to time. Such new versions will be similar in spirit to the present version, but may differ in detail to address new problems or concerns.

Each version is given a distinguishing version number. If the Library as you received it specifies that a certain numbered version of the GNU Lesser General Public License “or any later version” applies to it, you have the option of following the terms and conditions either of that published version or of any later version published by the Free Software Foundation. If the Library as you received it does not specify a version number of the GNU Lesser General Public License, you may choose any version of the GNU Lesser General Public License ever published by the Free Software Foundation.

If the Library as you received it specifies that a proxy can decide whether future versions of the GNU Lesser General Public License shall apply, that proxy's public statement of acceptance of any version is permanent authorization for you to choose that version for the Library.